



SGE GC Capillary Column innovation,  
manufacture and selection

74-82

100% Dimethyl Polysiloxane

BP1	83
BP1 PONA	84
BPX1	84

## GC Capillary Columns

100% Dimethyl Polysiloxane in a Sol-Gel Matrix

SolGel-1ms™	85
-------------	----

5% Phenyl / 95% Dimethyl Polysiloxane

BP5	86
-----	----

5% Phenyl Polysilphenylene-siloxane

BPX5	87-88
------	-------

5% Phenyl Polycarbosilane-siloxane

HT5	89
-----	----

8% Phenyl Polycarbosilane-siloxane

HT8	90
-----	----

35% Phenyl Polysilphenylene-siloxane

BPX35	90-91
-------	-------

35% Phenyl Polysilphenylene-siloxane

BPX608	91
--------	----

50% Phenyl Polysilphenylene-siloxane

BPX50	92
-------	----

70% Cyanopropyl Polysilphenylene-siloxane

BPX70	92-93
-------	-------

90% Cyanopropyl Polysilphenylene-siloxane

BPX90	93
-------	----

Polyethylene Glycol (PEG) in a Sol-Gel matrix

SolGel-WAX™	94
-------------	----

Polyethylene Glycol

BP20 (WAX)	94-95
------------	-------

Polyethylene Glycol (PEG) – TPA Treated

BP21 (FFAP)	95-96
-------------	-------

14% Cyanopropylphenyl Polysiloxane

BP10 (1701)	96
-------------	----

50% Cyanopropylphenyl Polysiloxane

BP225	97
-------	----

Cyanopropylphenyl Polysiloxane

BPX-VOLATILES	97
---------------	----

Cyanopropylphenyl Polysiloxane

BP624	98
-------	----

Permethylated Beta-Cyclodextrin (Chiral)

CYDEX-B™	98
----------	----

GC Applications by Industry

	99-146
--	--------

SGE's silica drawing towers where continuous lengths of fused silica are drawn and coated.

# GC Capillary Columns

GC Columns and Applications

- Five decades of capillary column innovation.
- End to end capillary column manufacture.
- Providing separation solutions.



## Five Decades of Capillary Column Innovation



SGE has a long history developing and producing GC capillary columns, with SGE's founder Ernest Dawes first being involved making glass capillary columns in 1959.

That expertise has been built upon with the development of leading capabilities in glass technology, polymer synthesis, surface chemistry and production processes all combined with an intimate knowledge of chromatography.

SGE develops and synthesizes specialty polymers leading to SGE being the first, and often only, capillary chromatography company to offer many types of GC stationary phases. SGE was the first to introduce the now industry standard silarylene phases in 1987 with their improved thermal stability, as well as SolGel in 1999 and the carborane phases in 1987. A detailed explanation of how these polymers work can be found on pages 76-80.

## End to End Capillary Column Manufacture

SGE has long been a manufacturer of GC capillary columns with the complete technology capability to produce the finest capillary columns from beginning to end, including the special requirements of producing the fused silica capillary tubing. This end to end manufacturing capability allows SGE to control the fabrication process precisely to produce the finest quality capillary columns available.

- Developing and synthesizing the specialty polymer stationary phases.
- Performing the specialty chemical treatment of the fused silica surface so that it is inert and compatible for the cross-linked stationary phase.
- Coating and cross-linking the polymer stationary phase.
- Quality testing of every completed capillary column to rigorous standards.

The individual technologies SGE employs in GC capillary column manufacture are:

- Drawing of the precision fused silica capillary tubing.

## Fused Silica

The process of producing fused silica at SGE is carried out on a series of sophisticated drawing towers with fine control of conditions and feedback loops to automatically make adjustments to the conditions. This ensures superb dimensional control and strength which is verified through stress proof testing of all material. By producing the fused silica ourselves, SGE has complete control of this important aspect of producing the highest quality GC capillary columns.

The fused silica used by SGE is very high purity devoid of impurities such as metal oxides found in conventional glasses. Depending on the application, SGE offers two types of FST coating - polyimide (max temp 400 °C) and aluminum (max. temperature 480 °C). SGE's capillary columns operate comfortably to 400 °C (dependent on the phase selected).

## Stationary Phase Polymer

SGE has designed its phase synthesis so that most capillary columns may be washed with solvent to remove any contamination. When a capillary column's performance has deteriorated from extended use or contamination, performance can often be restored through washing with a suitable solvent. See page 196 for details and equipment available for washing capillary columns.

## Rigorous Performance Testing

Test criteria are selected based on the applications that different capillary column types are targeted for, to ensure the capillary column meets the standards for that analysis. General purpose capillary columns are tested to ensure they meet inertness standards for difficult to chromatograph compounds, and run at conditions and levels designed to highlight variations in capillary column performance. For example, SGE's non-polar phase BPX5 is tested using active probes

such as n-decylamine and 2,4-dinitrophenol chromatographed at low concentrations (1-2 nanogram on capillary column for 0.25 µm film thickness) and with sufficient retained time on the run to induce tailing on all but the most highly inert capillary column. SGE does not offer separate ranges of capillary columns of different performance levels – all SGE GC capillary columns meet these high standards.

GC Columns and Applications

## Retention Time and Consistency

Because SGE controls the capillary column fabrication process from beginning to end we are also able to achieve remarkably consistent retention characteristics from column to column. When a method is established on an SGE column, the same separation can be expected column after column.

## Thermal Stability


A long term issue in capillary GC is the breakdown of the stationary phase in the capillary column at elevated temperatures which leads to rising and noisy baseline signals thereby limiting sensitivity of the analysis. Stationary phase breakdown at elevated temperatures cannot be eliminated but it can be reduced dramatically through improving the technology. SGE developed, and was the first to introduce, silarylene - containing polymers such as silphenylene stationary phases in 1987. Silphenylene phases replace some of the oxygen atoms in the backbone of the siloxane polymer with aromatic groups. This led to a dramatically improved thermal stability for GC phases with silphenylene phases now available in a wide range of polarities and selectivities. SGE capillary columns are monitored for bleed performance with rigorous standards established. Bleed is measured and specified in terms of detector signal and calibrated to "nanograms of siloxane per second" eluted from the capillary columns. **The test is performed at the maximum operating temperature for the capillary column.**



The measure for bleed of nanograms of siloxane per second eluting from the capillary column is more meaningful than exclusively reporting picoamp FID signal. Picoamp signal is highly dependent on the detector and conditions used and is not an

absolute measure. SGE carries out the bleed measurement on FID to assure the best performance possible.

Below is an example of the SGE GC Capillary Column Performance Report.

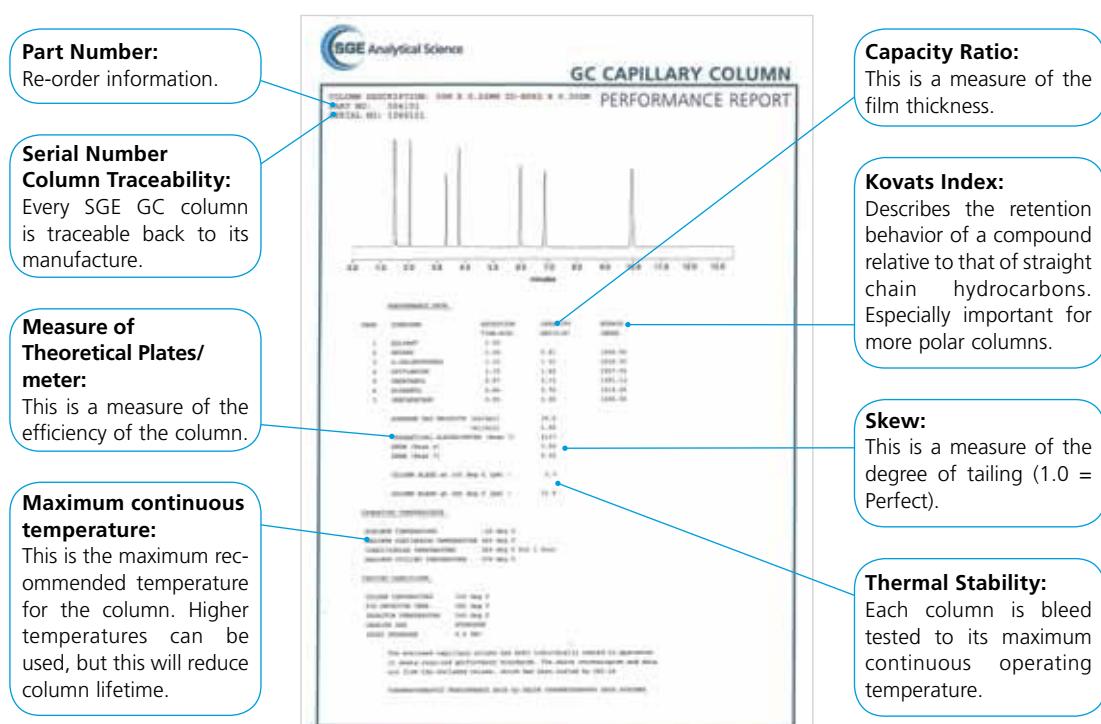

## Providing Separation Solutions

### GC Capillary Columns Polarity Scale

SGE strives to develop a better understanding of the interactions of the solute molecules with the GC stationary phase types in our product range and those we could design and synthesize. The objective is to be able to assist you the chromatographer to select a GC stationary phase for the separation of particular classes of compounds.

All chromatographers want the best separation and need to focus on the key parameters that influence the resolution equation. R can be viewed in three sections consisting of variables which influence capillary column efficiency, retention and selectivity.

$$R = \left( \frac{\sqrt{N}}{4} \right) \left( \frac{k}{k+1} \right) \left( \frac{\alpha-1}{\alpha} \right)$$

Column Efficiency      Retention      Selectivity

R = resolution, N = theoretical plates, k = capacity factor,  $\alpha$  = selectivity

Another way of viewing the resolution equation from the GC capillary column perspective is that quality impacts the capillary column efficiency, the physical dimensions of the capillary column influence retention and the phase chemistry dictates selectivity. Inevitably, many GC operators focus on flow rates and temperatures because of their importance in getting good peak shapes and nice separations – rarely do we pay attention to how the phase can have such an effect on the relative retention time. The fine detail of the chromatography comes in the interaction with the phase.


### Stationary Phase Polarity

A discussion on phase chemistry inevitably involves a reference to polarity – polarity in general terms and where phases fit along a linear polarity scale – but there is more

to it than this. There are different types of interactions based on the different types of functionality of the GC stationary phase polymer. In trying to create a scaled representation of the mechanisms of separation SGE has placed the stationary phases against a qualitative scale, although this scale is analyte dependent. The scale reflects the relative ability of phases to interact with particular types of analytes.

The scales shown in the 3D Phase Polarity diagram below, are qualitative rather than quantitative and have been derived from experimental work studying the retention of different analytes in the different types of stationary phases. Essentially the focus has been to develop a three dimensional representation of where each phase fits as a point on a plot of three classic bonding mechanisms - 'Van der Waals', H-bonding and  $\pi$ -bonding.

### 3D Phase Polarity Scale

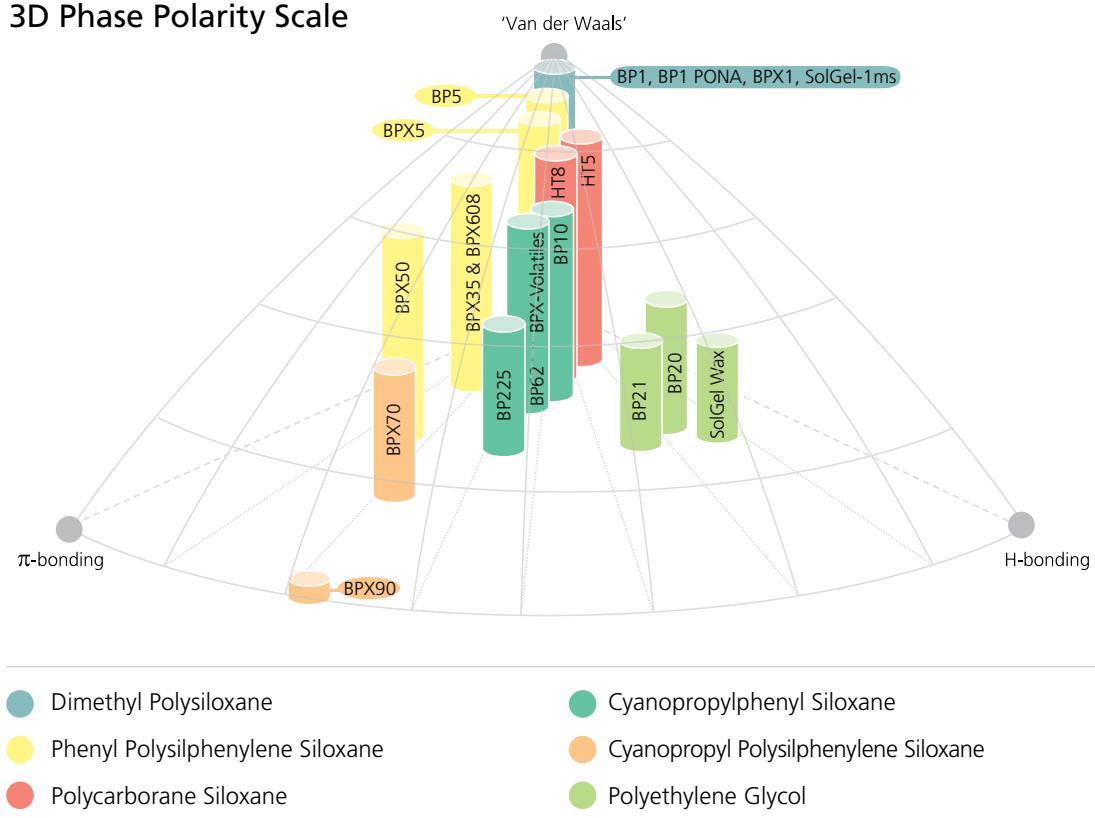

### Bonding Mechanisms

Van der Waals – essentially electrostatic attraction from temporary dipoles and are a very weak interaction. They are at their greatest relative contribution in the non-polar phases like the dimethylsiloxanes.

Hydrogen bonding results from the attraction of positive and negative charges of hydrogen and non-bonding pairs of electrons and is the force that holds water molecules together as liquid.

The  $\pi$ -bonding is associated with the aromatic class of compounds that include


benzene rings. Molecules with these loose clouds of donut shaped electronic charges have their own attraction towards each other. The  $\pi$ -bond in benzene is perpendicular to the benzene ring bonds so they interact more easily if the shape of the molecules does not create steric hindrance.

Stationary phases consist of basic polymer units with functionalities that can be modified by the addition of various moieties during synthesis. These moieties can be added in various amounts to create different concentrations of a particular functionality.



## SGE GC Capillary Column Phases

GC Columns and Applications

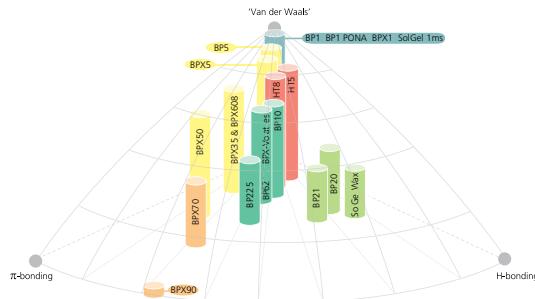


Color Code	Phase	Structure	SGE Phase	Characteristics
●	Dimethyl Polysiloxane	$\left[ \begin{array}{c} \text{CH}_3 & \text{CH}_3 \\   &   \\ \text{Si} - \text{O} - \text{Si} & - \text{O} \\   &   \\ \text{CH}_3 & \text{CH}_3 \end{array} \right]_n$	BP1 BP1 PONA BPX1 SolGel-1ms	<ul style="list-style-type: none"> <li>Polydimethylsiloxane (PDMS) "non-polar" type phases which rely on Van der Waals interactions between molecules and separate primarily based on "boiling point" type separation.</li> <li>Useful chromatographic space is usually considered in terms of modifications to non-polar retention. This is understandable because the GC is useful for volatile compounds and that usually means organics.</li> <li>Organics that can be vaporized are generally high in non-polar (alkane or hydrocarbon) character. It is this part of their surface that allows them to be soluble in a non-polar phase. It is also this characteristic that makes the BP1 (dimethylsiloxane) a universal phase.</li> </ul>
●	Diphenyl Dimethyl Siloxane (Phenyl substituted Siloxanes)	$\left[ \begin{array}{c} \text{O} & \text{O} \\   &   \\ \text{Si} - \text{O} & - \text{Si} - \text{O} \\   &   \\ \text{O} & \text{O} \end{array} \right]_n$ 95% 5%	BP5	<ul style="list-style-type: none"> <li>The classical 5% phenyl group of phases</li> </ul>
●	Phenyl Polysilphenylene Siloxane (Silphenylene substituted Polydimethylsiloxane)	$\left[ \begin{array}{c} \text{CH}_3 & \text{CH}_3 & \text{CH}_3 \\   &   &   \\ \text{O} & \text{Si} - \text{O} & \text{Si} - \text{O} \\   &   &   \\ \text{CH}_3 & \text{CH}_3 & \text{CH}_3 \end{array} \right]_y$	BPX5 BPX35 BPX608 BPX50	<ul style="list-style-type: none"> <li>Silphenylene phases have become fairly common now with many manufacturers offering at least some phases of this type, SGE has a full range.</li> <li>Phases with the "X" notation have a silphenylene backbone (exception is the BPX1).</li> <li>Phenyl substituted polymers are relatively non-polar and rely for their different functionality on <math>\pi</math> - bonding with the aromatic phenyl groups.</li> <li>SGE was the first GC capillary column manufacturer to introduce this type of phase commercially in the 1980s with the intention of improving the thermal stability to give higher maximum temperatures and reduced bleed.</li> </ul>
●	Polycarborene Siloxane	$\left[ \begin{array}{c} \text{O} & \text{O} \\   &   \\ \text{Si} - \text{O} & - \text{Si} - \text{O} \\   &   \\ \text{O} & \text{O} \end{array} \right]_n$ 	HT5 HT8	<ul style="list-style-type: none"> <li>The carborene phases were originally developed as very high thermal stability phases for high temperature work to 460 °C.</li> <li>The functionality of the carborenes is difficult to explain – they end up with pentavalent bonds with shared sigma bonds rather than <math>\pi</math> - bonds. The bonds are transient like a benzene with a ball of shared electrons.</li> <li>HT5 and HT8 are low <math>\pi</math>-bonding purely due to the low concentration of carborene in the polymer, otherwise it would be high.</li> </ul>
●	Cyanopropylphenyl Siloxane	$\left[ \begin{array}{c} \text{CN} & (\text{CH}_3)_3 \\   &   \\ \text{Si} - \text{O} & - \text{Si} - \text{O} \\   &   \\ \text{CH}_3 & \text{O} \end{array} \right]_x$	BP225 BP10 BP624 BPX-Volatiles	<ul style="list-style-type: none"> <li>'Polar' phases with &lt;50% cyanopropyl substituted dimethylpolysiloxane.</li> </ul>
●	Cyanopropyl Polysilphenylene Siloxane	$\left[ \begin{array}{c} \text{CH}_3 & \text{CH}_3 & \text{CH}_3 \\   &   &   \\ \text{O} & \text{Si} - \text{O} & \text{Si} - \text{O} \\   &   &   \\ \text{CH}_3 & \text{CH}_3 & \text{CH}_3 \end{array} \right]_y$	BPX70 BPX90	<ul style="list-style-type: none"> <li>High cyanopropyl substituted phases, are more difficult to make as efficient, thermally stable phases.</li> <li>BPX70 is equivalent to and behaves like a 70% cyanopropyl siloxane but with siphenyl end substituted backbone for stability which was introduced in 1987 and remained the most polar thermally stable phase for a long time.</li> <li>BPX90 which is equivalent to a 90% cyanopropyl siloxane and stable to 300 °C which is excellent for such a polar phase. The prominent interaction for BPX90 is <math>\pi</math> - <math>\pi</math> bonding with the cyano group; the cyano groups become almost entirely responsible for the partitioning.</li> </ul>
●	Polyethylene Glycol	$\left[ -\text{CH}_2 - \text{CH}_2 - \text{O} - \right]_n$	BP21 BP20 SolGel-WAX™	<ul style="list-style-type: none"> <li>(PEG) 'wax' type phases where the main separation mechanisms are hydrogen bonding or dipole interactions.</li> <li>The wax phases are often considered as ideal for mixtures of chemically different components such as those contained in essential oils.</li> </ul>

# Choosing the Right Phase for Your Separation

So how can you use this elaborate explanation of phases and bonding types?


The answer is simple! In separation science we seek solutions in resolving complex mixtures and a “one-phase fits all” is more a hope than a reality. Here SGE has explored different phases from a polarity scale to assist the chromatographer to choose the best combination of phases which provide an orthogonal solution rather than a simple variation of a theme.

Take for example the separation of aromatics on the polyethylene glycol capillary column BP20 (H-bonding) compared to BP1 where the primary interaction is Van der Waals. Whereas para- and meta-xylene are unresolved on BP1, they are clearly resolved on BP20 with a corresponding change in elution order to the alkanes. This is an interesting interaction because the aromatic xylenes have been attracted by the H-bond rich BP20. It is not a totally ‘one or the other’ situation when judging the contribution of H-bond and  $\pi$ -bond affinities, because they have some affinity for each other.

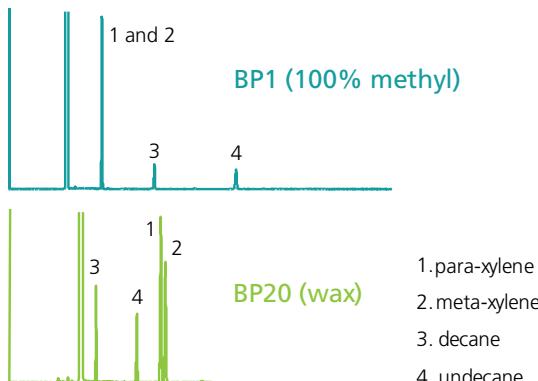

A higher component separation is demonstrated with a series of hydrocarbons run on a relatively non-polar phase (BPX5, on the x-axis in figure above right) and on a highly polar BPX90 with the retention times plotted on the y-axis. If the hydrocarbon family is split up on the basis of unsaturated

groups, this extra dimension shown in color (chemical group) reveals that the plot shows strong correlations for retention characteristics and functional chemistry.

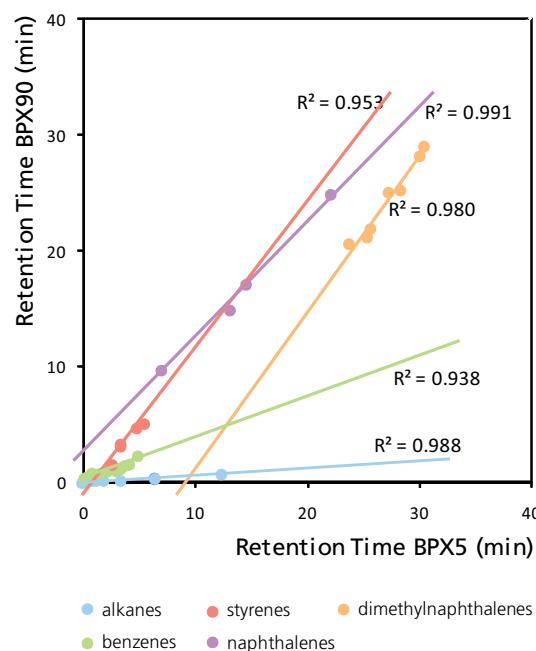

In this case, the hydrocarbon alkanes (light blue) are completely non-polar. They are retained on the phase only because the phase has sufficient non-polar character to interact with them. In the case of BPX90, it is so polar that it does not offer alkanes the opportunity for interaction. As a result, the alkanes tend to elute almost unretained. The alkanes show almost perfect orthogonality here. Retention on BPX5 versus no retention on BPX90 – they lie almost along the x-axis. We can now reason that if pure hydrocarbons (Van der Waals or non-polar interactions) give little or no BPX90 retention then retention of the remaining aromatics is due to purely  $\pi$  type interactions. When comparing GC phases, departures from the diagonal mark a significant change in the retention mechanism.

In conclusion, polar phases offer selectivity based on functionality rather than on Van der Waals interactions and are an ideal choice for the separation of analytes that were unresolved on non-polar or moderately polar phases.


# GC Capillary Columns

## GC Columns and Applications

- The primary advantages of considering phase selectivity include:
- 2D GC – the choice of orthogonal chemistries for the 1st and 2nd dimensions.
  - Fast GC – highly retained analytes on non-polar phases elute much earlier on polar phases.
  - Ubiquitous FAMEs methods.
  - Separation of unresolved analytes due to alternative functionality.


SGE hopes this information assists in your understanding of optimum GC capillary column phase selection for your application. Following is a summary of phase, plus other capillary column parameters such as internal diameter, capillary column length and film thickness, to assist with identification of the right SGE GC capillary column for your separation solution.

## GC Capillary Column Selection

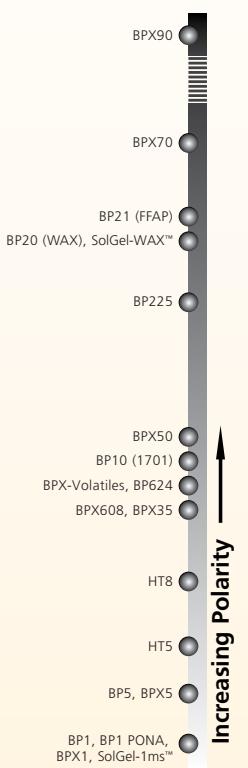

### 1. Stationary Phase

- Select the least polar phase that will perform the separation you require.
- Non-polar stationary phases separate analytes predominantly by order of boiling point. Increase the amount of phenyl and/or cyanopropyl content in the phase, and the separation is then influenced more by differences in dipole moments or charge distributions (BP10 (1701), BPX35, BPX50, BP225 and BPX70).

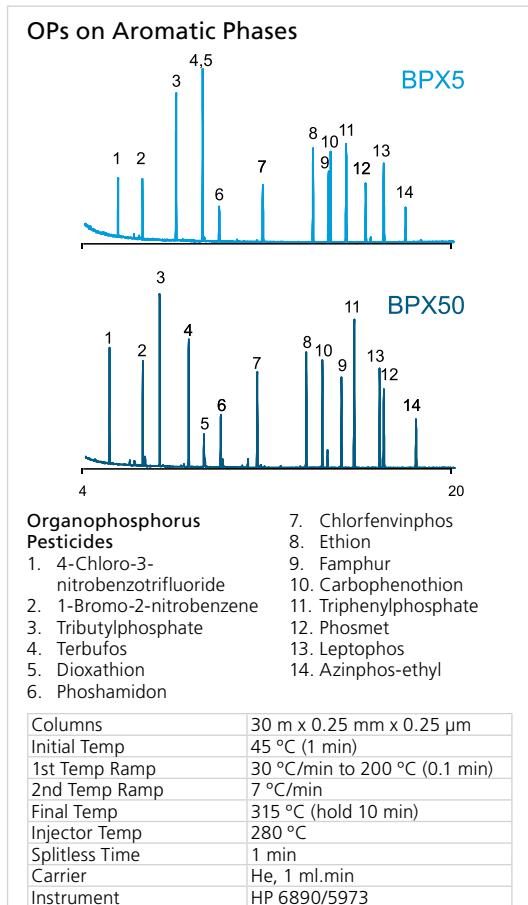


Effect of increasing Phenyl content in the stationary phase.

- To separate compounds that differ more in their hydrogen bonding capacities (for example aldehydes and alcohols), polyethylene glycol type phases are best suited - SolGel-WAX™, BP20 (WAX) and BP21(FFAP).

### 2. Internal Diameter

- The smaller the diameter the greater the efficiency, hence better resolution. Fast columns (0.1 mm ID) are used for faster analysis because the same resolution can be achieved in a shorter time.

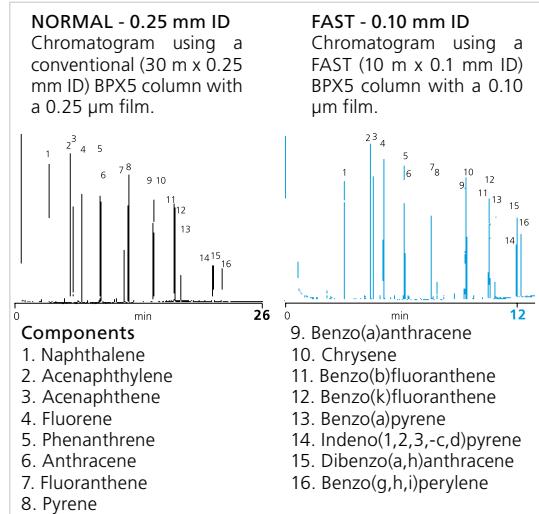

Effect of Internal Diameter. Polynuclear Aromatic Hydrocarbon (PAH) analysis.

### 3. Film Thickness

- For samples with a variation in solute concentration, a thicker film column is recommended. This will reduce the possibility of broad overloaded peaks co-eluting with other compounds of interest. If the separation of two solutes is sufficient and co-elution is still unlikely, even with large differences in concentration, then a thinner film can be used.
- The greater the film thickness the greater the retention of solutes, therefore the higher the elution temperature. As a rule, doubling the film thickness results in an increase in elution temperature of approximately 15-20 °C under isothermal conditions. Using a temperature program, the increase in elution temperature is slightly less.
- From the phase ratio value  $\beta$ , a column can be categorized for the type of application it would best suit. The smaller the  $\beta$  value, the greater the ratio of phase to the column inner diameter, making it better suited for analyzing volatile compounds.

Columns that have thin films are generally better suited for high molecular weight compounds and are characterized by large  $\beta$  values.

- Maintain phase ratio among different ID columns to yield similar chromatography.

GC Columns and Applications

$$\beta = \frac{id}{4d_f}$$


where

$\beta$  = phase ratio

$id$  = column internal diameter ( $\mu\text{m}$ )

$d_f$  = film thickness ( $\mu\text{m}$ )

Formula to calculate Phase Ratio.

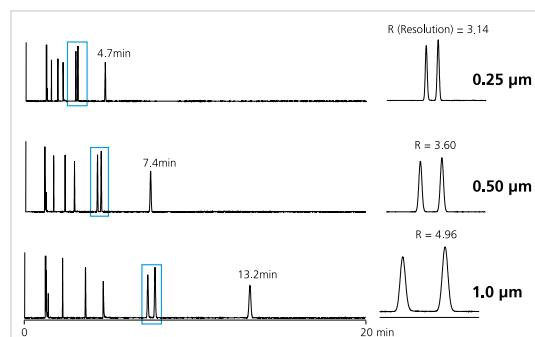


Film Thickness ( $\mu\text{m}$ )	100	150	220	250	320	530
0.10	250	-	550	625	800	1325
0.15	-	250	-	-	-	883
0.25	-	150	220	250	320	530
0.50	-	75	110	125	160	265
1.00	-	-	55	63	80	132
3.00	-	-	-	-	27	44
5.00	-	-	-	-	16	26

Table 1. Above shows the phase ratio ( $\beta$ ) available for the SGE range of capillary columns. Keeping a similar phase ratio when changing column internal diameters will ensure that your chromatographic parameters will not need substantial changes.

### 4. Column Length

- Always try to select the shortest column length that will provide the required resolution for the application. If the maximum column length available is being used and resolution of the sample mixture is still inadequate then try changing the stationary phase or internal diameter.
- Resolution is proportional to the square root of the column efficiency; therefore, doubling the column length will only increase the resolving power of the column by approximately 40%.

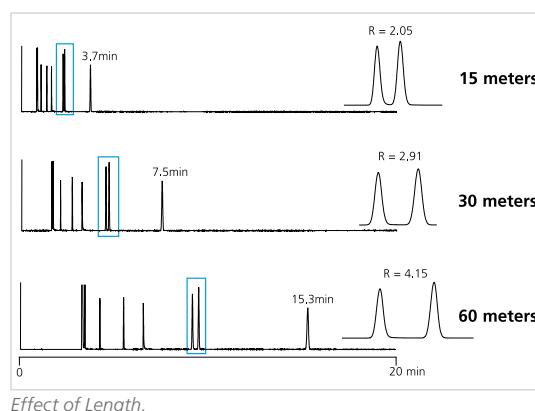

## Application Range For Varying Phase Ratios

Phase Ratio ( $\beta$ )	Application
16-100	Gases, Low M.W. Hydrocarbons, Solvents, Volatile Halogens (M.W.16-250)
100-320	Semi-volatiles, General Applications (M.W. 100-700)
320-1325	High M.W. Hydrocarbons, Waxes, Petroleum Products (M.W. 300-1500)


GC Columns and Applications

## SGE GC Capillary Column Phase Cross Reference Table

SGE Phase	Description	Capillary Column to Replace
BP1	100% Dimethyl Polysiloxane	DB-1, HP-1, Ultra-1, SPB-1, CP-Sil 5CB, RSL-150, RSL-160, Rtx®-1, ZB-1, CB-1, OV®-1, PE-1, 007-1(MS), SP-2100, SE-30, RH-1, CC-1, CP-Sil 5CB MS, VF-1ms, Petrocol DH
BP1-PONA	100% Dimethyl Polysiloxane	Petrocol DH, DB-Petro
BPX1	100% Dimethyl Polysiloxane	DB-HT Sim Dis, DB-2887, Rtx-2887, HP-1, Petrocol 2887, Petrocol EX2887
SolGel-1ms™	SolGel + 100% Dimethyl Polysiloxane	Unique highly inert phase
BP5	5% Phenyl Polysiloxane	DB-5, DB-5.625, Rtx-5, HP-5, Ultra-2, PTE-5, PB-5, MDN-5, CP-Sil 8CB, VB-5 & ZB-5
BPX5	5% Phenyl Polysilphenylene-siloxane	DB-5, DB-5ms, HP-5, Ultra-2, Rtx®-5, Rtx-5Sil MS, Rtx 5MS, AT-5, AT-5MS, 007-5MS, SPB-5, CP-Sil 8CB, VF-5ms, RSL-200, CB-5, OV®-5, PE-5, 007-2(MPS-5), SE-52, SE-54, XTI-5, PTE-5, CC-5, RH-5ms, ZB-5
BPX35	35% Phenyl Polysilphenylene-siloxane	DB-35, DB-35ms, Rtx-35, HP-35, HP-35MS, SPB-35, MDN-35, VB-50, ZB-35
BPX608	35% Phenyl Polysilphenylene-siloxane	DB-608, Rtx-35, SPB-608
BPX50	50% Phenyl Polysilphenylene-siloxane	OV-17, SP-2250, DB-17ms, DB-17ht, Rtx-50, SPB-50, HP-50+, HP-17, VB-50/608, ZB-50
HT5	5% Phenyl Polycarborene-siloxane	MXT-1 SimDist, HT-SimDist, DistCB, MXT-500
HT8	8% Phenyl Polycarborene-siloxane	No equivalent, unique high temperature capillary column with special selectivity (standard for PCB)
BP225	50% Cyanopropylphenyl Polysiloxane	HP-225, DB-225, Rtx-225
BP10 (1701)	14% Cyanopropylphenyl Polysiloxane	DB-1701, Rtx-1701, HP-1701, SPB-7, CP-Sil 19CB, VB-1701, ZB-1701
BP624, BPX-Volatiles	Cyanopropylphenyl Polysiloxane	DB-624, HP-VOC, Rtx Volatiles, Rtx 624, VOCOL, VB-624, ZB-624
BPX70	70% Cyanopropyl Polysilphenylene-siloxane	DB-23, CP-Sil 88, VF-23ms, SP-2330, SP-2380, Rtx®-2330, 007-23, AT-Silar, PE-23
BPX90	90% Cynopropyl Polysilphenylene-siloxane	Unique highly polar phase
BP21 (FFAP)	Polyethylene Glycol (TPA treated)	DB-FFAP, HP-FFAP, Stabilwax-DA, CP Wax 58CB, VB-FFAP, ZB-FFAP
BP20 (Wax)	Polyethylene Glycol	DB-Wax, Rtx-Wax, Stabilwax, HP20M, HP-Wax, HP-INNOWax, Supelcowax-10, AT-Wax, Nukol, CP Wax 2CB, VB-WAX, ZB-WAX
SolGel-WAX™	SolGel + Polyethylene Glycol	Unique highly inert phase
CYDEX-B	Permethylated Beta Cyclodextrin	Cyclodex-B, Rt-BDEXm

## Operating Temperature

For each SGE GC column phases temperature limits are represented three ways:

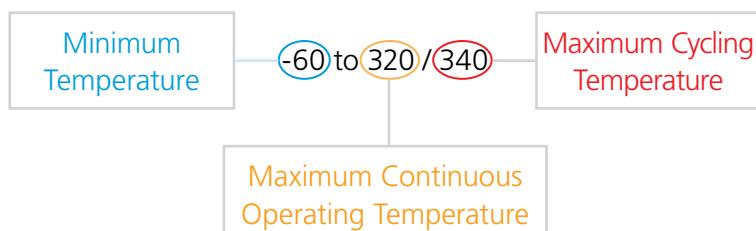

Minimum Temperature	Maximum Continuous Operating Temperature	Maximum Cycling Temperature
The temperature below which the capillary column will not separate components due to loss of partitioning in the stationary phase.	The maximum temperature at which a capillary column can be held for 72 hours with no significant change. SGE capillary columns are designed to pass all criteria measured by their test analysis after 72 hours at their Maximum Continuous Operating Temperature.	The maximum cycling temperature to which a capillary column can be taken for short periods (up to 30 minutes) without causing serious bleed problems or degradation of the phase. This is usually higher than the Maximum Continuous Operating Temperature. The lifetime of a capillary column is affected by the amount of time it spends at high temperatures.

# GC Capillary Columns | 100% Dimethyl Polysiloxane

## BP1

- Classic crosslinked dimethyl polysiloxane technology.
- Excellent general purpose GC column.
- Low bleed.
- Non-polar.
- Suitable for all routine analyses.
- 320 – 340 °C upper temperature limit – dependent on film thickness.

Especially Suitable for these Industries:	 Fuels  Environment  Forensics
Application Areas:	Suitable for analysis of hydrocarbons, aromatics, pesticides, phenol, herbicides, amines. Applications AMI04, POL05, PHA04.
Suitable Replacement for:	DB-1, DB-Petro, HP-1, HP-1MS, Rtx-1, Ultra-1, SPB-1, SPB-1 Sulfur, Petrocol DH, CP-Sil 5CB, VB-1, ZB-1, VF-1ms.

GC Columns and Applications

### Expert Tip :

Columns should be conditioned to the maximum continuous temperature unless specified.




ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits (°C)	Part No.
0.1	0.1	10	-60 to 320/340	054022
0.15	0.25	12	-60 to 320/340	054028
0.15	0.25	25	-60 to 320/340	054029
0.22	0.1	12	-60 to 320/340	054040
0.22	0.25	12	-60 to 320/340	054046
0.22	1	12	-60 to 320/340	054052
0.22	0.25	15	-60 to 320/340	054049
0.22	0.1	25	-60 to 320/340	054041
0.22	0.25	25	-60 to 320/340	054047
0.22	1	25	-60 to 320/340	054053
0.22	0.25	30	-60 to 320/340	054050
0.22	0.1	50	-60 to 320/340	054042
0.22	0.25	50	-60 to 320/340	054048
0.22	1	50	-60 to 320/340	054054
0.22	0.25	60	-60 to 320/340	054051
0.25	0.1	15	-60 to 320/340	054039
0.25	0.25	15	-60 to 320/340	054043
0.25	0.25	30	-60 to 320/340	054044
0.25	0.5	30	-60 to 320/340	054820
0.25	1	30	-60 to 320/340	054056
0.25	0.25	60	-60 to 320/340	054045
0.25	0.5	60	-60 to 320/340	054812
0.25	1	60	-60 to 320/340	054815
0.32	0.25	12	-60 to 320/340	054058
0.32	0.5	12	-60 to 320/340	054064
0.32	1	12	-60 to 320/340	054070
0.32	0.25	15	-60 to 320/340	054061
0.32	0.25	25	-60 to 320/340	054059
0.32	0.5	25	-60 to 320/340	054065
0.32	1	25	-60 to 320/340	054071
0.32	4	25	-60 to 280/300	054076
0.32	5	25	-60 to 280/300	054081
0.32	0.25	30	-60 to 320/340	054062
0.32	0.5	30	-60 to 320/340	054068
0.32	1	30	-60 to 320/340	054813
0.32	1.5	30	-60 to 300/320	054811
0.32	3	30	-60 to 300/320	054073
0.32	4	30	-60 to 280/300	054077
0.32	0.25	50	-60 to 320/340	054060
0.32	0.5	50	-60 to 320/340	054066
0.32	1	50	-60 to 320/340	054072
0.32	5	50	-60 to 280/300	054082
0.32	0.25	60	-60 to 320/340	054067

## GC Columns and Applications

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
0.32	0.5	60	-60 to 320/340	054069
0.32	1	60	-60 to 320/340	054810
0.32	5	60	-60 to 280/300	054085
0.53	1	12	-60 to 320/340	054086
0.53	3	12	-60 to 300/320	054097
0.53	0.5	15	-60 to 320/340	054870
0.53	1	15	-60 to 320/340	054089
0.53	1	25	-60 to 320/340	054087
0.53	3	25	-60 to 300/320	054098
0.53	5	25	-60 to 280/300	054095
0.53	0.5	30	-60 to 320/340	054092
0.53	1	30	-60 to 320/340	054090
0.53	2.6	30	-60 to 300/320	054819
0.53	3	30	-60 to 300/320	054808
0.53	5	30	-60 to 280/300	054806
0.53	1	50	-60 to 320/340	054088
0.53	5	50	-60 to 280/300	054096
0.53	0.5	60	-60 to 320/340	054871
0.53	3	60	-60 to 300/320	054809
0.53	5	60	-60 to 280/300	054807

## BP1 PONA




- Designed for the analysis of petroleum products.
- Non-polar phase for PONA analysis.
- Detailed hydrocarbon analysis according to ASTM (DHA-method).
- Crosslinked and washable.
- Very high resolving power columns for complex samples.
- 320 – 340 °C upper temperature limit.

Especially Suitable for this Industry:	
Application Areas:	Suitable for petroleum hydrocarbons, gasoline range hydrocarbons, MTBE, paraffins, olefins, naphthenes, aromatics. Application PET01.
Suitable Replacement for:	Petrocol DH, DB-Petro, HP-PONA, AT-Petro, Elite-PONA, ZB-1, 007-1-100-0.5F, Rtx-1PONA, CP Sil PONA.

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
0.15	0.5	50	-60 to 320/340	054950
0.25	0.5	100	-60 to 320/340	054818

## BPX1



- Non-polar column.
- Dimensionally stabilized phase.
- Low bleed.
- Specifically designed for high temperature hydrocarbon analysis.
- Ideal for simulated distillation methods (ASTM Method D2887).
- 430 °C upper temperature limit – Aluminum clad.
- 370- 400 °C upper temperature limit – Polyimide clad (dependent on film thickness).

Especially Suitable for this Industry:	
Application Areas:	ASTM methods D2887 and D6532. Applications PET26, PET18, ENV54.
Suitable Replacement for:	DB-2887, DB-HT Sim Dis, HP-1, Petrocol 2887, Petrocol EX2887, Rtx-2887.

## BPX1

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
<b>Polyimide Clad</b>				
0.1	0.1	10	-30 to 400/400	054777
0.53	2.65	6	-30 to 370/370	0548025
0.53	0.1	10	-30 to 400/400	054803
0.53	0.9	10	-30 to 400/400	054801
0.53	2.65	10	-30 to 370/370	054802
<b>Aluminum Clad</b>				
0.53	0.1	5	-30 to 430/430	054800
0.53	0.17	5	-30 to 430/430	054782
0.53	0.1	10	-30 to 430/430	054779


GC Columns and Applications

## GC Capillary Columns | 100% Dimethyl Polysiloxane in a Sol-Gel Matrix

### SolGel-1ms™


#### What is Sol-Gel?

Sol-Gel is essentially a synthetic glass with ceramic-like properties. These modified Sol-Gels offer the best of both worlds – ceramic-like properties with the film-forming properties of the associated polymer. The Sol-Gel process involves hydrolysis and condensation of alkoxides that lead to the formation of a glassy material at ambient temperatures. This method has been used to produce high quality ceramics and mono- and multi-component glasses of high homogeneity and purity. The further modification of this ceramic material with polymeric material (with appropriate functionality) leads to the formation of organic-inorganic nanomaterials.



#### Conventional Phase

The phase is coated onto the surface of the fused silica resulting in weak intermolecular bonding but no covalent bonding, ie no anchoring.



#### Sol-Gel Phase

Anchored to the surface of the fused silica through covalent bonding.

#### Where can Sol-Gel materials be used?

The further organic-modified Sol-Gels have been incorporated in a variety of high-end technology products including membrane chemical and pH sensors, films for protection of optical lenses, cosmetic and electronic products.

#### SGE and Sol-Gel materials?

At SGE, Sol-Gel processes are used to manufacture stationary phases for gas chromatography capillary columns. SGE is the first company to offer Sol-Gel technology capillary columns. The organic component in our case is a GC stationary phase. The final Sol-Gel product has all the properties of the GC phase as well as the additional properties of the Sol-Gel part. The Sol-Gel material is able to covalently bond to the surface of the fused silica. The 'heavy-duty' bonding imparts better thermal stability of the phase leading to ultra-low bleed capillary columns. To date, two Sol-Gel phases have been developed by SGE, namely SolGel-1ms™ and SolGel-WAX™. The SolGel-1ms™ stationary phase is a non-polar phase derived from 100% dimethyl polysiloxane. SolGel-WAX™ is a polar phase which incorporates polyethylene glycol in the matrix.

#### Expert Tip :

Always use SilTite™ or SilTite™ Finger-Tite ferrules when connecting a column to a GC/MS interface.



SolGel-1ms™ has a robust, inert, high temperature, non-polar phase for use with mass spectrometers.

- Highly inert.
- Less bleed means:
  - Better MS library identification.
  - Less ion source maintenance.
  - Better sensitivity.
- Can also be used for all non-MS detectors.
- Same selectivity as BP1.
- 340 /360 °C upper temperature limit.

## GC Columns and Applications

Especially Suitable for these Industries:	 Fuels  Environment  Forensics
Application Areas:	Recommended for highly active compounds. Applications ARO14, ENV51.
Operating Temperature:	0.25 µm film thickness 0 °C to 340/360 °C.
Suitable Replacement for:	DB-1, DB-Petro, HP-1, HP-1MS, Rtx-1, Ultra-1, SPB-1, SPB-1 Sulfur, Petrocol DH, CP-Sil 5CB, VB-1, ZB-1, VF-1ms.

ID (mm)	Film Thickness (µm)	Length (m)	Temperature Limits (°C)	Part No.
0.25	0.25	30	0 to 340/360	054795
0.25	0.25	60	0 to 340/360	054793
0.32	0.25	30	0 to 340/360	054798
0.32	0.25	60	0 to 340/360	054794

## GC Capillary Columns | 5% Phenyl / 95% Dimethyl Polysiloxane

## BP5

- Excellent general purpose GC column.
- Low bleed.
- Non-polar.
- High temperature.
- 320/340 °C upper temperature limit - dependent on film thickness.

Especially Suitable for these Industries:	 All Industries
Application Areas:	General purpose, aromatics, pesticides, herbicides, drugs of abuse, hydrocarbons, solvent impurities, PCB congeners or Aroclor mixes, essential oils, semivolatiles. Applications FOO02, AMI03, PHA08, PHA 10.
Suitable Replacement for:	DB-5, Rtx-5, HP-5, Ultra-2, PTE-5, SPB-5, MDN-5, CP-Sil 8CB, VB-5, ZB-5.

For your instrument specific septa see the Instrument Quick Pick Guide on pages 167-180.

ID (mm)	Film Thickness (µm)	Length (m)	Temperature Limits (°C)	Part No.
0.22	0.25	12	-60 to 320/340	054167
0.22	0.25	25	-60 to 320/340	054168
0.22	0.25	30	-60 to 320/340	054171
0.22	0.25	50	-60 to 320/340	054169
0.22	1	50	-60 to 320/340	054175
0.25	0.25	15	-60 to 320/340	054182
0.25	0.25	30	-60 to 320/340	054183
0.25	0.5	30	-60 to 320/340	054202
0.25	1	30	-60 to 320/340	054203

## BP5

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
0.25	0.25	60	-60 to 320/340	054184
0.25	1	60	-60 to 320/340	054215
0.32	0.25	12	-60 to 320/340	054179
0.32	0.25	15	-60 to 320/340	054176
0.32	0.25	25	-60 to 320/340	054180
0.32	0.5	25	-60 to 320/340	054186
0.32	1	25	-60 to 320/340	054192
0.32	0.25	30	-60 to 320/340	054177
0.32	0.5	30	-60 to 320/340	054216
0.32	1	30	-60 to 320/340	054189
0.32	0.5	50	-60 to 320/340	054187
0.32	1	50	-60 to 320/340	054193
0.32	0.25	60	-60 to 320/340	054178
0.32	1	60	-60 to 320/340	054188
0.53	1	12	-60 to 320/340	054197
0.53	1	15	-60 to 320/340	054194
0.53	1.5	15	-60 to 320/340	054199
0.53	1	25	-60 to 320/340	054198
0.53	0.5	30	-60 to 320/340	0541935
0.53	1	30	-60 to 320/340	054195
0.53	5	30	-60 to 280/300	054196
0.53	1.5	60	-60 to 280/300	054204

GC Columns and Applications


### Expert Tip :

If the injection port temperature is not specified in the method, 250 °C is usually the recommended temperature.



## GC Capillary Columns | 5% Phenyl Polysilphenylene-siloxane

### BPX5



- High temperature.
- General purpose GC column – suitable for over 80% of all routine analyses performed by gas chromatography.
- Very low bleed – ideal for trace analysis.
- Non-polar.
- Extremely inert.
- Ideal for GC-MS.
- 360 – 370 °C upper temperature limit – dependent on film thickness.

Recommended column for General Purpose use.

Especially Suitable for these Industries:	All Industries
Areas:	Ultra trace analyses, pesticides/herbicides, hydrocarbons, solvents, phenols, amines, GC/MS and other specific detector applications. Applications ENV62, ARO09, ENV20, ENV03, ENV48, ENV59, ENV84, FOO21, FLA14, FLA16, FLA15, FLA12 FLA13, ENV54, PET22, SOL33 PHA06, PHA08, PHA15.
Suitable Replacement for:	DB-5, DB-5ms, DB-5.625, XTI-5, Rtx-5ms, Ultra-2, HP-5, HP-5MS, HP5-TA, SPB-5, MDN-5S, CP-Sil8CB, Rxt-Sil 5MS, AT-5ms, VB-5, ZB-5, VF-5ms.




ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
0.1	0.1	10	-40 to 360/370	054099
0.15	1.2	10	-40 to 360/370	054106
0.15	0.25	12	-40 to 360/370	054103
0.15	0.4	12	-40 to 360/370	054107
0.15	0.25	25	-40 to 360/370	054104
0.15	0.4	25	-40 to 360/370	054108

## GC Columns and Applications

## Expert Tip :


If you're having problems with solvent focusing, or early eluting peaks seem broad or lopsided in splitless injection, then try using a column with a thicker film.

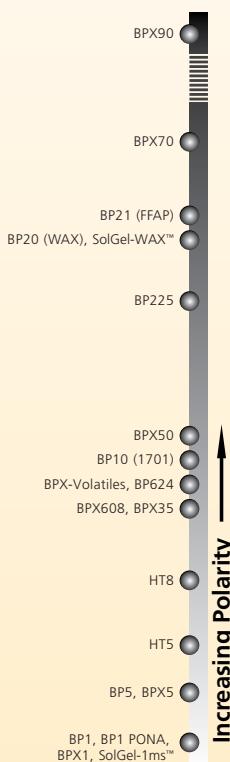

## BPX5

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits (°C)	Part No.
0.15	0.15	30	-40 to 360/370	054110
0.15	0.25	50	-40 to 360/370	054105
0.18	0.18	40	-40 to 360/370	054229
0.22	0.25	12	-40 to 360/370	054112
0.22	0.25	25	-40 to 360/370	054113
0.22	1	25	-40 to 360/370	054116
0.22	0.25	30	-40 to 360/370	054142
0.22	0.25	50	-40 to 360/370	054114
0.22	1	50	-40 to 360/370	054117
0.25	0.25	7	-40 to 360/370	054149
0.25	0.1	15	-40 to 360/370	0542170
0.25	0.25	15	-40 to 360/370	054100
0.25	1	15	-40 to 360/370	054121
0.25	0.1	30	-40 to 360/370	0541011
0.25	0.25	30	-40 to 360/370	054101
0.25	0.5	30	-40 to 360/370	0541025
0.25	1	30	-40 to 360/370	054122
0.25	0.25	60	-40 to 360/370	054102
0.25	1	60	-40 to 360/370	054123
0.32	1	6	-40 to 360/370	0541261
0.32	0.25	12	-40 to 360/370	054118
0.32	0.5	12	-40 to 360/370	054124
0.32	1	12	-40 to 360/370	054127
0.32	0.25	15	-40 to 360/370	054144
0.32	1	15	-40 to 360/370	054152
0.32	0.25	25	-40 to 360/370	054119
0.32	0.5	25	-40 to 360/370	054125
0.32	1	25	-40 to 360/370	054128
0.32	3	25	-40 to 350/360	054136
0.32	0.25	30	-40 to 360/370	054145
0.32	0.5	30	-40 to 360/370	0541205
0.32	1	30	-40 to 360/370	054153
0.32	0.25	50	-40 to 360/370	054120
0.32	0.5	50	-40 to 360/370	054126
0.32	1	50	-40 to 360/370	054129
0.32	0.25	60	-40 to 360/370	054146
0.32	1	60	-40 to 360/370	054154
0.53	0.25	12	-40 to 360/370	054133
0.53	1	12	-40 to 360/370	054130
0.53	3	12	-40 to 350/360	054138
0.53	0.5	15	-40 to 360/370	0541344
0.53	1	15	-40 to 360/370	054147
0.53	1.5	15	-40 to 350/360	0541347
0.53	3	15	-40 to 350/360	054159
0.53	0.25	25	-40 to 360/370	054134
0.53	1	25	-40 to 360/370	054131
0.53	3	25	-40 to 350/360	054139
0.53	0.5	30	-40 to 360/370	0541345
0.53	1	30	-40 to 360/370	054148
0.53	1.5	30	-40 to 350/360	0541348
0.53	3	30	-40 to 350/360	054160
0.53	1	50	-40 to 360/370	054132
0.53	1	60	-40 to 360/370	054158

## HT5



GC Columns and Applications

- Ultra high temperature columns.
- Unique phase – no equivalent phases.
- Ideal for simulated distillation applications (petroleum industry).
- 460/480 °C upper temperature limit – Aluminum clad.
- 380/400 °C upper temperature limit – Polyimide clad.
- Bonded and cross-linked.
- Able to be solvent rinsed.

Especially Suitable for these Industries:	Fuels  Environment  Food
Application Areas:	Simulated distillation, general hydrocarbon profiles, pesticides/herbicides, GC/MS applications. Applications FOO16, PET11, PET27, PET06.
Suitable Replacement for:	MXT-1 Sim Dist, HT-Sim, DistCB, MXT-500.


ID (mm)	Film Thickness (µm)	Length (m)	Temperature Limits (°C)	Part No.
<b>Polyimide Clad</b>				
0.22	0.1	12	10 to 380/400	054631
0.22	0.1	25	10 to 380/400	054632
0.25	0.1	15	10 to 380/400	054633
0.25	0.1	30	10 to 380/400	054634
0.32	0.1	12	10 to 380/400	054641
0.32	0.5	15	10 to 380/400	054667
0.32	0.1	25	10 to 380/400	054642
0.32	0.5	30	10 to 380/400	054668
0.53	0.1	6	10 to 380/400	054655
0.53	0.5	10	10 to 380/400	054670
0.53	0.15	12	10 to 380/400	054657
0.53	0.5	15	10 to 380/400	054671
0.53	0.15	25	10 to 380/400	054658
0.53	0.5	30	10 to 380/400	054672
<b>Aluminum Clad</b>				
0.22	0.1	12	10 to 460/480	054635
0.22	0.1	25	10 to 460/480	054636
0.32	0.1	12	10 to 460/480	054651
0.32	0.1	25	10 to 460/480	054652
0.32	0.1	50	10 to 460/480	054653
0.53	0.075	5	10 to 460/480	054673
0.53	0.1	6	10 to 460/480	054661
0.53	0.15	12	10 to 460/480	054662
0.53	0.15	25	10 to 460/480	054665

**Expert Tip :**  
To prevent increasing retention times in your chromatography, replace the septum regularly.



For your  
gas purifiers  
see pages  
165-166.


# GC Capillary Columns | 8% Phenyl Polycarborene-siloxane



## HT8

- High temperature.
- Low bleed.
- Preferred column for polychlorinated biphenyl (PCB) compounds.
- Separates PCB's on ortho ring substitution as well as boiling point.
- Ideal for environmental analysis.
- 360/370 °C upper temperature limit.
- Unique high temperature phase suited for the analysis of persistent organic pollutants (POPs).

GC Columns and Applications

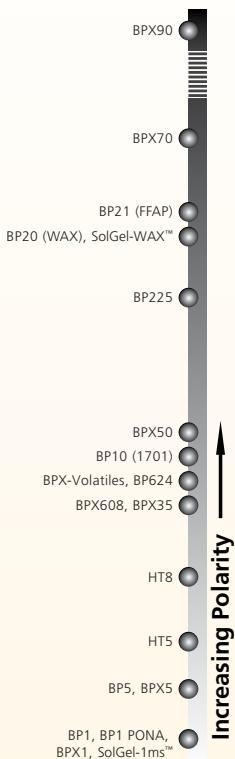

Especially Suitable for this Industry:	Environment
Application Areas:	PCB congener analyses, nitro-substituted aromatics, polynuclear aromatic hydrocarbons, pesticides/herbicides. Application ARO08.
Suitable Replacement for:	No equivalents, unique ultra high temperature column.

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits (°C)	Part No.
0.1	0.1	10	-20 to 360/370	054690
0.22	0.25	12	-20 to 360/370	054674
0.22	0.25	25	-20 to 360/370	054675
0.22	0.25	50	-20 to 360/370	054676
0.25	0.25	30	-20 to 360/370	054677
0.25	0.25	60	-20 to 360/370	054683
0.32	0.25	12	-20 to 360/370	054679
0.32	0.25	25	-20 to 360/370	054680
0.32	0.25	50	-20 to 360/370	054681
0.32	0.25	60	-20 to 360/370	054682
0.53	0.5	12	-20 to 360/370	054684
0.53	0.5	25	-20 to 360/370	054685

# GC Capillary Columns | 35% Phenyl Polysilphenylene-siloxane

## BPX35

- Mid polarity column.
- Ideal for confirmational analysis.
- Inert.
- Equivalent to USP phase G42.
- High temperature.
- Very low bleed.
- Pharmaceutical specialist.
- 330/360 °C upper temperature limit.
- Bonded and cross-linked.
- Able to be solvent rinsed.

Especially Suitable for these Industries:	Pharmaceuticals    Environment    Food    Forensics
Application Areas:	Environmental analyses, pesticides/herbicides, drugs of abuse, pharmaceuticals, polynuclear aromatic hydrocarbons, GC/MS applications. Applications ENV57, ENV04 AMI09, ALC09, SOL25, PHA14, PHA09
Suitable Replacement for:	DB-35, DB-35ms, Rtx-35, HP-35, HP-35MS, SPB-35, MDN-35.

## BPX35

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
0.1	0.1	10	10 to 330/360	054699
0.22	0.25	15	10 to 330/360	054713
0.22	0.25	25	10 to 330/360	054711
0.22	0.25	30	10 to 330/360	054714
0.22	0.25	50	10 to 330/360	054712
0.25	0.25	15	10 to 330/360	054700
0.25	1	15	10 to 330/360	054703
0.25	0.25	30	10 to 330/360	054701
0.25	0.5	30	10 to 330/360	0547025
0.25	1	30	10 to 330/360	054704
0.25	0.25	60	10 to 330/360	054702
0.25	1	60	10 to 330/360	054705
0.32	0.25	15	10 to 330/360	054723
0.32	0.5	15	10 to 330/360	054718
0.32	1	15	10 to 330/360	054716
0.32	0.25	25	10 to 330/360	054721
0.32	0.25	30	10 to 330/360	054724
0.32	0.5	30	10 to 330/360	0547158
0.32	1	30	10 to 330/360	054717
0.32	0.25	50	10 to 330/360	054722
0.53	0.5	15	10 to 330/360	054734
0.53	1	15	10 to 330/360	054736
0.53	0.5	30	10 to 330/360	054735
0.53	1	30	10 to 330/360	054737

GC Columns and Applications

### Expert Tip :


When peak shape deteriorates, replace the liner immediately and cut 30cm from the front end of the column.



## GC Capillary Columns | 35% Phenyl Polysilphenylene-siloxane

### BPX608

- Optimized for ECD.
- Ideal for organochlorine, pesticides and herbicides analysis.
- Maximum temperature 370 °C.

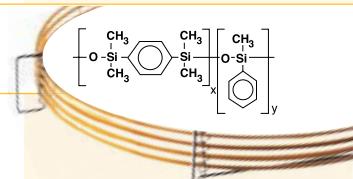


Especially Suitable for these Industries:	
Application Areas:	Environmental analyses, EPA 608, pesticides/herbicides.
Operating Temperature	10 °C to 360/370 °C.
Suitable Replacement for:	DB-608, Rtx-35, SPB-608, HP-35, ZB-35.

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
0.32	0.4	25	10 to 360/370	054823

For your instrument specific septa see the Instrument Quick Pick Pages pages 167-180.



# GC Capillary Columns | 50% Phenyl Polysilphenylene-siloxane



## BPX50

GC Columns and Applications

- Mid polarity.
- Inert.
- Low bleed.
- High temperature.
- Ideal for a range of EPA methods and pharmaceutical applications.

- 330/350 °C upper temperature limit.
- Bonded and cross-linked.
- Able to be solvent rinsed.

Especially Suitable for these Industries:	
Application Areas:	EPA methods 604, 608, 8060, 8081, triazines/herbicides, drug screening, steroids and a variety of pharmaceutical applications GC2D. Applications ENV62, ENV45, ENV65, PHA19.
Suitable Replacement for:	OV-17, SP-2250, DB-17, DB-17ms, DB-17ht, Rtx-50, SPB-50, HP-50+, HP-17.

### Expert Tip :

When installing your column into an FID jet, never pass the column through the flame. This will burn the inner (phase) and outer (polyimide) coatings and will cause higher background signals.



## GC Capillary Columns | 70% Cyanopropyl Polysilphenylene-siloxane

## BPX70

- High temperature.
- Custom designed for separation of Fatty Acid Methyl Esters (FAMEs).
- Industry standard column for FAME analysis.
- Polar phase.
- Long operating life.
- 250/260 °C upper temperature limit.
- Bonded and cross-linked.
- Able to be solvent rinsed.

Especially Suitable for these Industries:	
Application Areas:	Fatty acid methyl esters (FAMEs), carbohydrates, pharmaceuticals, GC/MS applications. Applications FOO02, FOO04.
Suitable Replacement for:	DB-23, Rtx-2330, SP-2330, CP-Sil 88, SP2380, HP-23.

## BPX70

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
0.1	0.2	10	50 to 250/260	054600
0.22	0.25	12	50 to 250/260	054601
0.22	0.25	25	50 to 250/260	054602
0.22	0.25	30	50 to 250/260	054612
0.22	0.25	50	50 to 250/260	054603
0.22	0.25	60	50 to 250/260	054613
0.25	0.25	15	50 to 250/260	054621
0.25	0.25	30	50 to 250/260	054622
0.25	0.25	60	50 to 250/260	054623
0.25	0.25	120	50 to 250/260	054624
0.32	0.25	12	50 to 250/260	054605
0.32	0.25	25	50 to 250/260	054606
0.32	0.25	30	50 to 250/260	054616
0.32	0.25	50	50 to 250/260	054607
0.32	0.25	60	50 to 250/260	054617
0.53	0.5	15	50 to 250/260	054619
0.53	0.5	25	50 to 250/260	054610
0.53	0.5	30	50 to 250/260	054620

GC Columns and Applications


### Expert Tip :

Set the FID temperature 20 °C above the maximum method temperature.



## GC Capillary Columns | 90% Cyanopropyl Polysilphenylene-siloxane

### BPX90

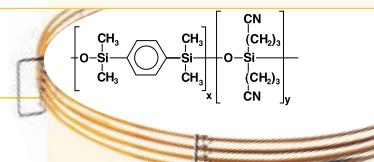

- Unique bonded phase.
- Highly polar.
- Thermally stable.
- Excellent resolution for cis and trans isomers.
- 260/280 °C upper temperature limit.
- Able to be solvent rinsed.


Especially Suitable for these Industries:	General Chemistry  Fuels  Environment  Food
Application Areas:	Ideal for fast separation of fragrances, aromatics, petrochemical, pesticides, PCBs and isomers of Fatty Acid Methyl Esters (FAMEs). Application AN0022C.
Suitable Replacement for:	Unique to SGE.

For your  
gas purifiers  
see page  
165-166.

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
0.25	0.25	15	80 to 260/280	054570
0.25	0.25	30	80 to 260/280	054580
0.25	0.25	60	80 to 260/280	054590
0.25	0.25	100	80 to 260/280	054596
0.32	0.5	15	80 to 260/280	054573
0.32	0.5	30	80 to 260/280	054583
0.32	0.5	60	80 to 260/280	054593



# GC Capillary Columns | Polyethylene Glycol (PEG) in a Sol-Gel matrix



GC Columns and Applications

## SolGel-WAX™

- The world's highest temperature wax phase.
- Bonded polyethylene glycol.
- Very robust high-temperature column.
- Less susceptible to damage by oxygen than conventional wax phases.
- Polar phase.
- Low bleed and inert.
- 280 °C upper temperature limit.
- Bonded and cross-linked.
- Able to be solvent rinsed.

Especially Suitable for these Industries:	 General Chemistry  Food
Application Areas:	Recommended for highly active compounds. Applications ARO13, FLA19, FLA22, FLA21, FLA18, POL06, ENV52.
Suitable Replacement for:	DB-Wax, Rtx-Wax, Stabilwax, HP20M, HP-Wax, HP-INNOWax, Supelcowax-10, AT-Wax, Nukol, CP Wax 52CB, VB-WAX, ZB-WAX.

ID (mm)	Film Thickness (µm)	Length (m)	Temperature Limits (°C)	Part No.
0.1	0.1	10	30 to 260/280	0547100
0.25	0.25	30	30 to 260/280	054796
0.25	1	30	30 to 260/280	054787
0.25	0.25	60	30 to 260/280	054791
0.32	0.25	30	30 to 260/280	054788
0.32	0.5	30	30 to 260/280	054797
0.32	0.25	60	30 to 260/280	054789
0.32	0.5	60	30 to 260/280	054792
0.53	0.5	30	30 to 260/280	054786
0.53	1	30	30 to 260/280	054785

## GC Capillary Columns | Polyethylene Glycol




## BP20 (WAX)

- Industry standard wax column.
- Polar phase.
- 240 – 280 °C upper temperature limit – dependent on film thickness.
- Bonded and cross-linked.
- Able to be solvent rinsed.

Especially Suitable for these Industries:	 General Chemistry  Environment  Food
Application Areas:	Alcohol, free acids, fatty acid methyl esters (FAMEs), aromatics, solvents, essential oils. Applications FOO03, FOO24 FLA03, ALC03, ACI03, POL01, PHA13.
Suitable Replacement for:	DB-Wax, HP-20M, Supelcowax 10, CB-Wax, Stabilwax, Carbowax, HP-Innowax, Rtx-WAX, PE-WAX, RH-WAX, ZB-WAX, TRWAX.

## BP20 (WAX)

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
0.1	0.1	10	20 to 260/280	054405
0.22	0.25	12	20 to 260/280	054420
0.22	0.25	25	20 to 260/280	054421
0.22	0.25	30	20 to 260/280	054424
0.22	0.25	50	20 to 260/280	054422
0.22	0.25	60	20 to 260/280	054425
0.25	0.25	15	20 to 260/280	054426
0.25	0.25	30	20 to 260/280	054427
0.25	0.5	30	20 to 260/280	054415
0.25	1	30	30 to 240/260	054439
0.25	0.25	60	20 to 260/280	054428
0.25	0.5	60	20 to 260/280	054458
0.32	0.25	15	20 to 260/280	054432
0.32	0.25	25	20 to 260/280	054430
0.32	0.5	25	20 to 260/280	054436
0.32	1	25	20 to 240/260	054442
0.32	0.25	30	20 to 260/280	054433
0.32	0.5	30	20 to 260/280	054438
0.32	1	30	30 to 240/260	054444
0.32	0.25	50	20 to 260/280	054431
0.32	0.5	50	20 to 260/280	054437
0.32	1	50	20 to 240/260	054443
0.32	0.25	60	20 to 260/280	054434
0.32	0.5	60	20 to 260/280	054457
0.32	1	60	20 to 240/260	054445
0.53	1	12	20 to 240/260	054447
0.53	2	12	20 to 240/260	054455
0.53	0.5	15	20 to 260/280	054961
0.53	1	15	20 to 240/260	054450
0.53	1	25	20 to 240/260	054448
0.53	2	25	30 to 240/260	054456
0.53	0.5	30	20 to 260/280	054440
0.53	1	30	20 to 240/260	054451
0.53	0.5	60	20 to 260/280	054963
0.53	1	60	20 to 240/260	0544515

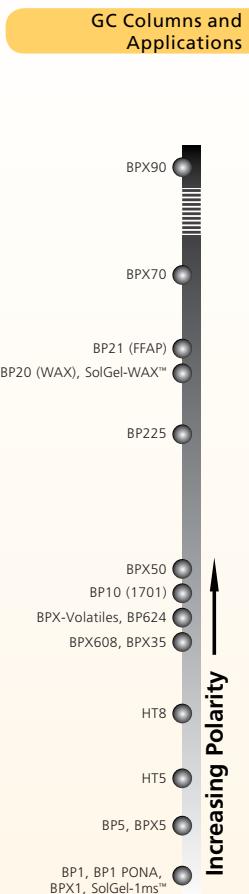

## GC Capillary Columns | Polyethylene Glycol (PEG) – TPA Treated

### BP21 (FFAP)

- Nitroterephthalic acid modified PEG.
- Polar phase.
- Ideal for low molecular weight acids.
- 240/250 °C upper temperature limit.
- Able to be solvent rinsed (water or methanol is NOT recommended for rinsing).
- Bonded and cross-linked.

Especially Suitable for these Industries:	 General Chemistry  Environment  Food
Application Areas:	Volatile free acids, fatty acid methyl esters, alcohols, aldehydes, acrylates, ketones. Applications ACI02, SOL04.
Suitable Replacement for:	DB-FFAP, HP-FFAP, Stabilwax-DA, CPWax-58CB.




## GC Columns and Applications

## BP21 (FFAP)

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
0.22	0.25	25	35 to 240/250	054462
0.22	0.25	50	35 to 240/250	054463
0.25	0.25	15	35 to 240/250	054464
0.25	0.25	30	35 to 240/250	054465
0.25	0.25	60	35 to 240/250	054466
0.32	0.25	12	35 to 240/250	054467
0.32	0.25	15	35 to 240/250	054470
0.32	0.25	25	35 to 240/250	054468
0.32	0.25	30	35 to 240/250	054471
0.32	0.25	50	35 to 240/250	054469
0.32	0.25	60	35 to 240/250	054472
0.32	0.5	50	35 to 240/250	054480
0.53	0.5	12	35 to 240/250	054473
0.53	0.5	15	35 to 240/250	054476
0.53	0.5	25	35 to 240/250	054474
0.53	0.5	30	35 to 240/250	054477
0.53	1	30	35 to 240/250	054478

## GC Columns | 14% Cyanopropylphenyl Polysiloxane



## BP10 (1701)

- Used for organochlorine pesticides analysis.
- Highly inert.
- Low bleed.
- 260/300 °C upper temperature limit - dependent on film thickness.
- Bonded and cross-linked.
- Able to be solvent rinsed.

Especially Suitable for these Industries:			
Application Areas:	Environmental analyses (EPA methods 608 and 8081), pesticides/herbicides, drugs of abuse, pharmaceuticals.		
Suitable Replacement for:	DB-1701, Rtx-1701, SPB-7, HP-1701, CP-Sil 19CB, 007-1701, PE-1701, SP-1701.		

ID (mm)	Film Thickness ( $\mu\text{m}$ )	Length (m)	Temperature Limits ( $^{\circ}\text{C}$ )	Part No.
0.22	0.25	12	-20 to 280/300	054252
0.22	0.25	25	-20 to 280/300	054253
0.22	0.25	50	-20 to 280/300	054254
0.25	0.25	15	-20 to 280/300	054255
0.25	0.25	30	-20 to 280/300	054256
0.25	1	30	-20 to 260/280	054271
0.25	0.25	60	-20 to 280/300	054257
0.32	0.25	15	-20 to 280/300	054258
0.32	0.5	15	-20 to 280/300	054264
0.32	0.25	25	-20 to 280/300	054262
0.32	0.5	25	-20 to 280/300	054268
0.32	0.25	30	-20 to 280/300	054259
0.32	0.5	30	-20 to 280/300	054265
0.32	1	30	-20 to 260/280	054270
0.32	0.5	50	-20 to 280/300	054269
0.32	0.25	60	-20 to 280/300	054260
0.32	0.5	60	-20 to 280/300	054266
0.53	1	15	-20 to 260/280	054282
0.53	1	25	-20 to 260/280	054280
0.53	1	30	-20 to 260/280	054283

## Expert Tip :

Do not use plastic tubing in GC systems. Plastic tubing, when used for general plumbing, can absorb up to 20% moisture allowing external laboratory gases to permeate through the tubing. SGE recommends clean stainless steel tubing to be used throughout the GC system.



# GC Columns | 50% Cyanopropylphenyl Polysiloxane

## BP225

- Mid to high polarity.
- Low bleed.
- Bonded and cross-linked.
- 230/260 °C upper temperature limit.
- Able to be solvent rinsed.

GC Columns and Applications

Especially Suitable for these Industries:	 
Application Areas:	Fatty Acid Methyl Esters (FAMEs), carbohydrates, neutral sterols.
Suitable Replacement for:	DB-225, HP-225 and RTX-225.

ID (mm)	Film Thickness (µm)	Length (m)	Temperature Limits (°C)	Part No.
0.22	0.25	25	40 to 230/260	054352
0.22	0.25	50	40 to 230/260	054353
0.32	0.25	25	40 to 230/260	054358
0.53	0.5	25	40 to 230/260	054364

For your instrument specific septa see the Instrument Quick Pick Guide pages 167-180.

# GC Columns | Cyanopropylphenyl Polysiloxane


## BPX-VOLATILES

- Polar phase.
- EPA volatile organics analysis (EPA 624, 502.2, SW-846 8240/8260).
- 290/300 °C upper temperature limit.
- Able to be solvent rinsed.
- Bonded and cross-linked.

Especially Suitable for these Industries:	  
Application Areas:	Environmental analyses, volatile organics, alcohol analysis, USP G43. Application TP-0102-C.
Suitable Replacement for:	DB-VRX, HP-624, OPTIMA 624, ELITE-624, 007-624, RTX-VOLATILES, SPB-624, TRV1, CPSIL 13 CB, VOCOL, VB-624, CP-624.

ID (mm)	Film Thickness (µm)	Length (m)	Temperature Limits (°C)	Part No.
0.18	1	20	0 to 290/300	054978
0.18	1	40	0 to 290/300	054979
0.25	1.4	30	0 to 290/300	054980
0.25	1.4	60	0 to 290/300	054981
0.32	1.8	30	0 to 290/300	054982
0.32	1.8	60	0 to 290/300	054983
0.53	3	30	0 to 290/300	054984
0.53	3	60	0 to 290/300	054985

# GC Columns | Cyanopropylphenyl Polysiloxane



## BP624

GC Columns and Applications

- US EPA 624 optimized column.
- Designed for volatiles analysis.
- Ideal for EPA624, SW-846 methods 8240/8260.
- Ideal for USP G43 method.
- 230/240 °C upper temperature limit.
- Able to be solvent rinsed.
- Bonded and cross-linked.

Especially Suitable for these Industries:	
Application Areas:	EPA method 624, drinking water volatiles, chlorinated hydrocarbons, solvents, Excellent for U.S. EPA Methods: 501.3, 502.2, 503.1, 524.2, 601, 602, 8010, 8015, 8020, 8240, 8260. Applications ENV17, ENV13.
Suitable Replacement for:	DB-624, OV-624, AT-624, HP-VOC, CP-Select624CB, 007-624, Rtx-Volatiles, Rtx 624, VOCOL, ZB-624.

ID (mm)	Film Thickness (µm)	Length (m)	Temperature Limits (°C)	Part No.
0.22	1.2	25	0 to 230/240	054826
0.22	1.2	30	0 to 230/240	054827
0.25	1.4	15	0 to 230/240	054839
0.25	1.4	30	0 to 230/240	054840
0.25	1.4	60	0 to 230/240	054842
0.32	1.8	25	0 to 230/240	054830
0.32	1.8	30	0 to 230/240	054832
0.32	1.8	50	0 to 230/240	054831
0.32	1.8	60	0 to 230/240	054841
0.53	3	25	0 to 230/240	054834
0.53	3	30	0 to 230/240	054836
0.53	3	50	0 to 230/240	054835
0.53	3	60	0 to 230/240	054838

# GC Columns | Permethylated Beta-Cyclodextrin (Chiral)

## CYDEX-B™

- Separation of chiral compounds

Especially Suitable for these Industries:	 
Application Areas:	Separation of enantiomeric compounds found in natural products. Application FLA05.
Operating Temperature:	30 °C to 220/240 °C
Suitable Replacement for:	Cyclodex-B, Rt-BDEXm, LIPODEX C


ID (mm)	Film Thickness (µm)	Length (m)	Temperature Limits (°C)	Part No.
0.22	0.25	25	30 to 220/240	054900
0.22	0.25	50	30 to 220/240	054901
0.32	0.25	25	30 to 220/240	054902

# GC Application by Industry | Environmental

## ENV 62 | Polynuclear Aromatic Hydrocarbons (PAH) Analysis on BPX50

Column Part No.:	054751
Phase:	BPX50, 0.25 µm film
Column:	30 m x 0.25 mm ID
(PAH) standard:	10 ng/ µL in dichloromethane
Initial Temp.:	65 °C, 0.5 min
Rate 1.:	25 °C/min to 140 °C
Rate 2.:	10 °C/min to 325 °C
Final Temp.:	325 °C, 15 min
Detector Type:	MSD
Carrier Gas:	Helium, 9.7 psi
Carrier Gas Flow:	1.1 mL/min constant

Flow:	On
Average Linear Velocity:	39 cm/sec at 65 °C
Mode of Injection:	splitless
Purge on Time:	0.5 min.
Purge on (split) Vent Flow:	60 mL/min
Injection Volume:	0.2 µL
Injection Temp.:	250 °C
Autosampler:	No
Liner Type:	4 mm ID Double Taper
Liner Part Number:	092018

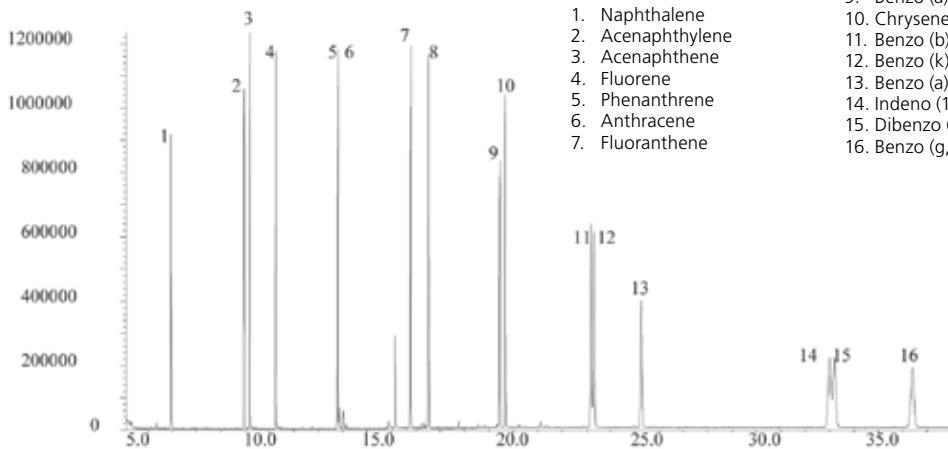


### Components

- 1. Naphthalene
- 2. Acenaphthylene
- 3. Acenaphthene
- 4. Fluorene
- 5. Phenanthrene
- 6. Anthracene
- 7. Fluoranthene
- 8. Pyrene
- 9. Benzo (a) anthracene
- 10. Chrysene
- 11. Benzo (b) fluoranthene
- 12. Benzo (k) fluoranthene
- 13. Benzo (a) pyrene
- 14. Indeno (1,2,3-c,d) pyrene
- 15. Dibenzo (a,h) anthracene
- 16. Benzo (g,h,i) perylene

## ARO 08 | Analysis of Polynuclear Aromatic Hydrocarbons on HT8

Column Part No.:	054462
Phase:	HT8, 0.25 µm film
Column:	25 m x 0.22 mm ID
Initial Temp.:	150 °C, 1 min

Rate:	4 °C/min
Final Temp.:	380 °C, 5 min
Carrier Gas:	He, 20 psi
Detector:	FID

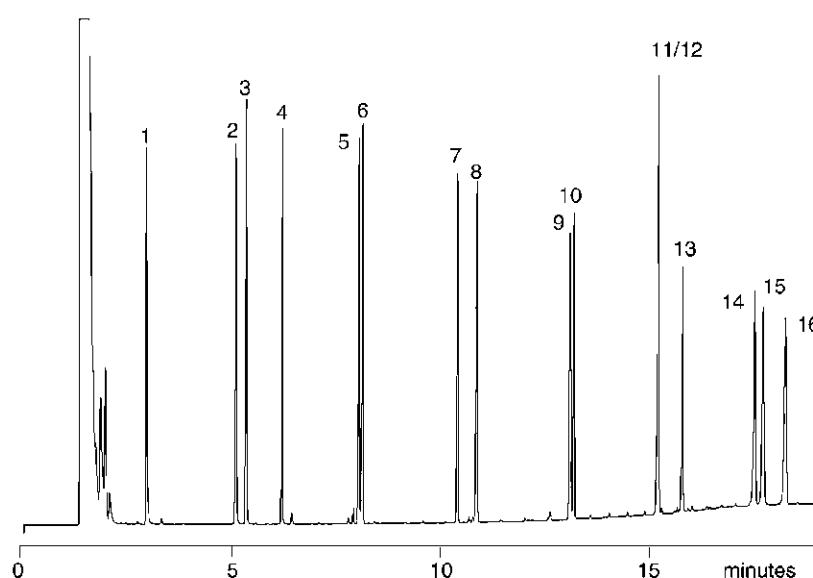


11/12

### Components

- 1. Naphthalene
- 2. Acenaphthylene
- 3. Acenaphthene
- 4. Fluorene
- 5. Phenanthrene
- 6. Anthracene
- 7. Pyrene
- 8. Fluoranthene
- 9. Benzo (a) anthracene
- 10. Chrysene
- 11. Benzo (b) fluoranthene
- 12. Benzo (k) fluoranthene
- 13. Benzo (a) pyrene
- 14. Indeno (1,2,3-c,d) pyrene
- 15. Dibenzo (a,h) anthracene
- 16. Benzo (g,h,i) perylene




GC Columns and Applications

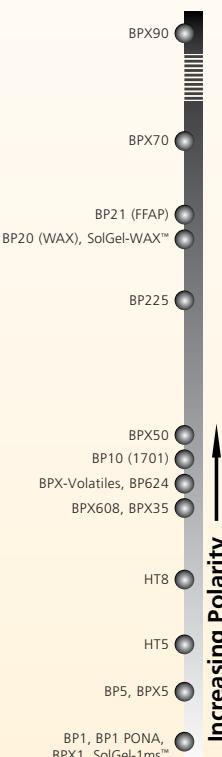




## AP 0040C | HT8: The Perfect PCB Column

Separation of CB31 &amp; CB28

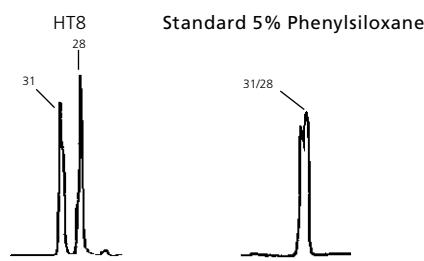

Chromatogram on the left clearly demonstrates the significant difference in selectivity of the HT8 column. By GC/MS, quantitation of CB28 using a standard 5% phenylpolysiloxane column is impossible as coelution with CB31 (with the same number of chlorines) occurs.

HT8 separates the two congeners by a full minute allowing quantitation to be performed with ease.

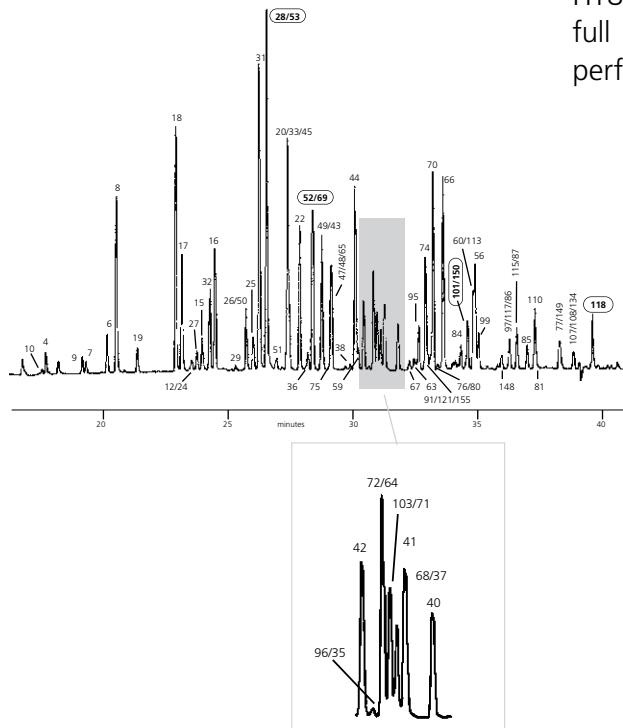

## AROCLOL 1242

**Column Part No.: 054676**

Phase: HT8, 0.25 µm film

Column: 50 m x 0.22 mm ID

Initial Temp: 80 °C, 2 min

Rate 1: 30 °C/min

Temp 2: 170 °C



Rate 2: 3 °C/min

Final Temp: Split, 300 °C

Carrier Gas: He, 40 psi

Detector: ECD, 330 °C

Congener #	CI Position	CI #	Identification by GC/MS
42	23-24	4	✓
96	236-26	5	✓
35	34-3	3	✓
64	235-4	4	✗
72	25-35	4	✓
103	246-25	5	✓
71	26-34	4	✓
41	234-2	4	✓
68	24-35	4	✓
37	34-4	3	✓
100	246-24	5	✓

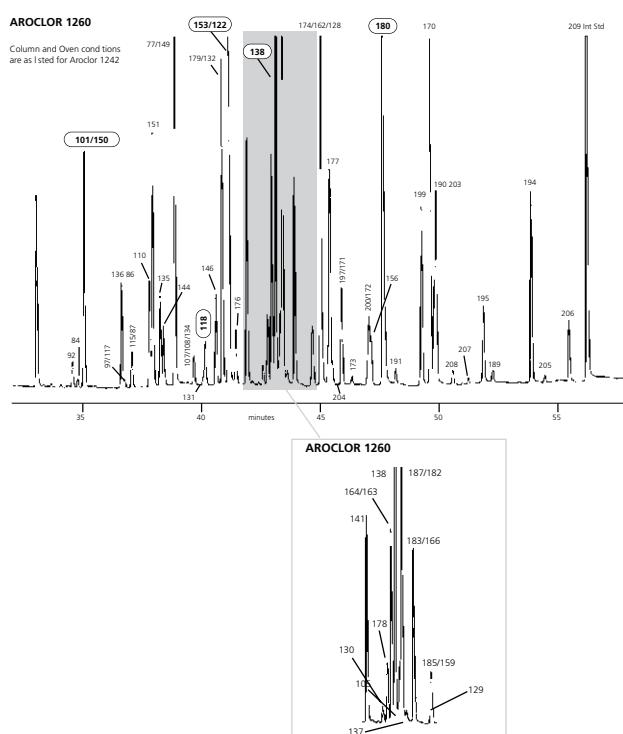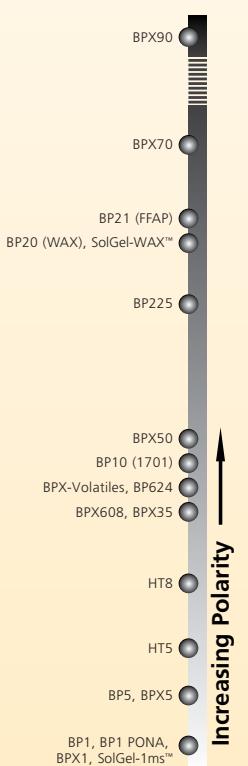


Congener #	CI Position	CI #	Identification by GC/MS
42	23-24	4	✓
96	236-26	5	✓
35	34-3	3	✓
64	235-4	4	✗
72	25-35	4	✓
103	246-25	5	✓
71	26-34	4	✓
41	234-2	4	✓
68	24-35	4	✓
37	34-4	3	✓
100	246-24	5	✓

## TP-0187-C | Analysis of Polynuclear Aromatic Hydrocarbons on BPX50




GC Columns and Applications

Column Part No.:	054701	Temperature Profile:	
Phase:	BPX50, 0.25 µm film	Hold 70 °C for 1 min	
Column:	30 m x 25 µm ID	70 °C to 140 °C at 25 °C/min	
Gas Flow:	1.5 ml/min Helium	140 °C to 250 °C at 15 °C/min	
Injection:	Split 1 µl (1 ng on column)	250 °C to 310 °C at 4 °C/min	
Injection Temperature:	250°C	Hold 310 °C for 8 min	

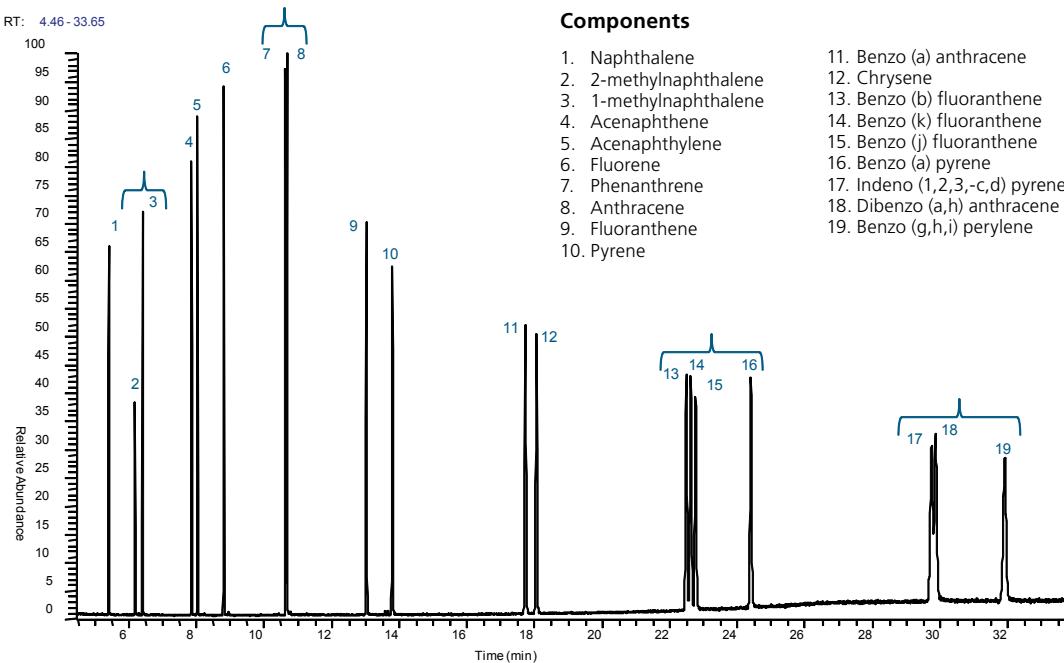

## ENV 17 | Analysis of 16 Volatile Compounds in Drinking Water on BP624

Column Part No.:	054826	Final Temp.:	170 °C
Phase:	BP624, 1.2 µm	Detector:	HP5870 MSD
Column:	25 m x 0.22 mm ID	Injection Mode:	Splitless
Initial Temp.:	50 °C, 2 min	Carrier Gas:	He, 15 psi
Rate:	15 °C/min		

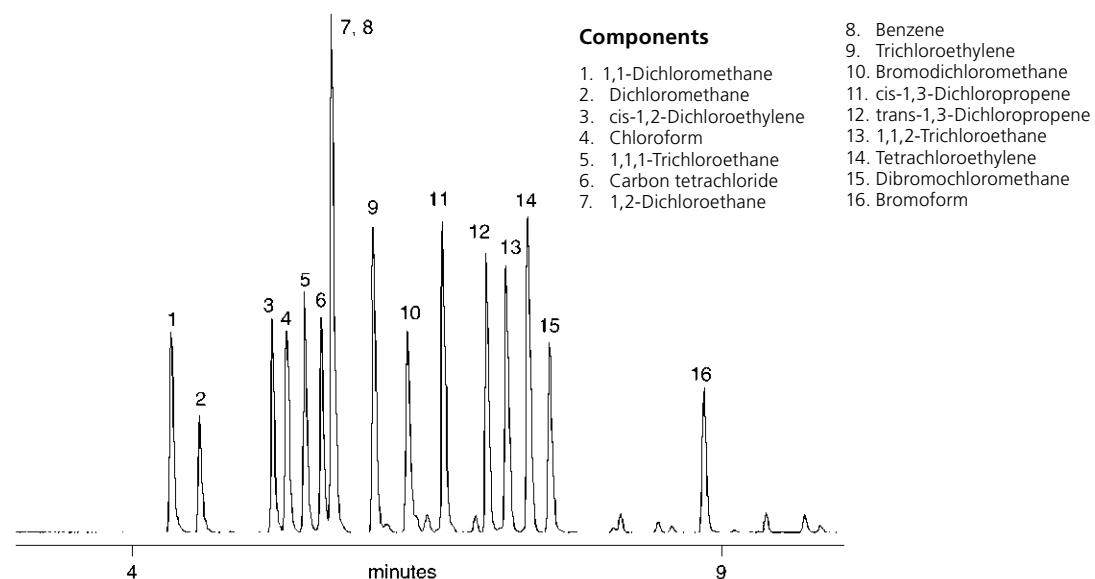




## ENV 13 | Analysis of Volatiles from Drinking Water on BP624

Column Part No.:	054835	Rate 2:	15 °C/min
Phase:	BP624, 3.0 µm	Final Temp.:	210 °C, 1 min
Column:	50 m x 0.53 mm ID	Detector:	MSD, MJSC Jet Separator
Initial Temp.:	35 °C, 2 min	Injection Mode:	Purge & Trap
Rate 1:	8 °C/min	Carrier Gas:	He, 10 ml/min
Temp 2:	180 °C, 5 min		

Note: Column which provides fast analysis of all EPA compounds. BP624 is also ideal for the analysis of many commonly used solvents.

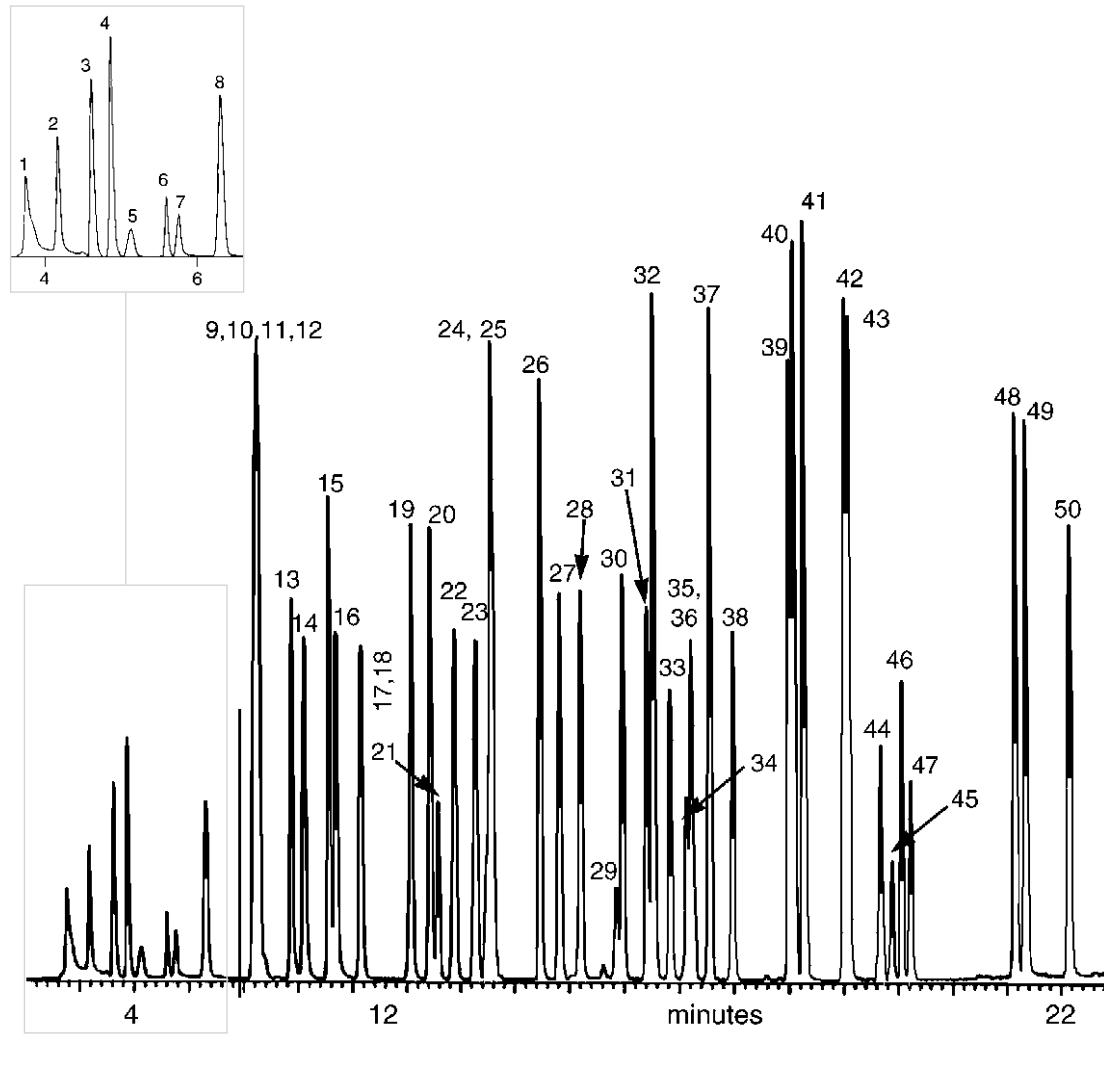**Components**

1. Carbon dioxide
2. Dichlorodifluoromethane
3. Chloromethane
4. Vinyl chloride
5. Acetaldehyde
6. Bromomethane
7. Chloroethane
8. Trichlorofluoroethane
9. Trichloroethane
10. Acrolein
11. Acetone
12. 1,1-Dichloroethene
13. Carbon disulfide
14. Methylene chloride
15. trans-1,2-Dichlorethane
16. Acrylonitrile




17. 1,1-Dichloroethane
18. Vinyl acetate
19. 2-Butanone (MEK)
20. cis-1,2-Dichloroethene
21. Bromochloromethane (Int. Std.)
22. 1,1-Trichloroethane
23. Carbon tetrachloride
24. 1,2-Dichloroethane-d4 (Surrogate)
25. 1,2-Dichloroethane
26. Trichloroethene
27. 1,2-Dichloroethene
28. Bromodichloromethane
29. 4-Methyl-2-pentanone
30. cis-1,3-Dichloropropene
31. Toluene-(d8) (Surrogate)
32. Toluene
33. trans-1,3-Dichloropropene
34. 2-Bromo-1-chloropropane (Int.Std)
35. 1,1,2-Trichlorethane
36. 2-Hexanone
37. Tetrachloroethene
38. Dibromochloromethane
39. Chlorobenzene
40. Ethylbenzene
41. m,p-Xylene
42. o-Xylene
43. Styrene
44. Bromoform
45. 1,4-Dichlorobutane (Int. Std)
46. Bromofluorobenzene
47. 1,1,2,2- Tetrachloroethene
48. 1,3-Dichlorobenzene
49. 1,4-Dichlorobenzene
50. 1,2-Dichlorobenzene

# TP-0102-C | Analysis of Volatile Organic Pollutants on a Volatiles GC Column



GC Columns and Applications

<b>Column Part No.:</b>	<b>054979</b>	Average Linear Velocity:	35 cm/sec at 40 °C
<b>Phase:</b>	<b>BPX-Volatiles 1µm film</b>	Injection Mode:	Split
<b>USEPA 502.2 mix:</b>	<b>200 ppm in Methanol</b>	Split Ratio:	50:1
<b>Column:</b>	<b>40m x 0.18mm ID</b>	Injection Volume:	1 µL
Initial Temp:	40 °C, 0 min.	Injection Temperature:	250 °C
Rate 1:	6 °C to 210 °C	Autosampler:	No
Rate 2:	15 °C to 250 °C	Liner Type:	4 mm ID Single Taper
Final Temp:	250 °C, 5 min	Liner Part Number:	092017
Detector Type:	Mass Spectrometer	Column Part Number:	054979
Carrier Gas:	He, 40.3 psi	ms-NoVent™ Part no.:	113400
Carrier Gas Flow:	1.2 µL/min.	HP5973 restrictor:	113409
Constant Flow:	On	Full scan	45-450

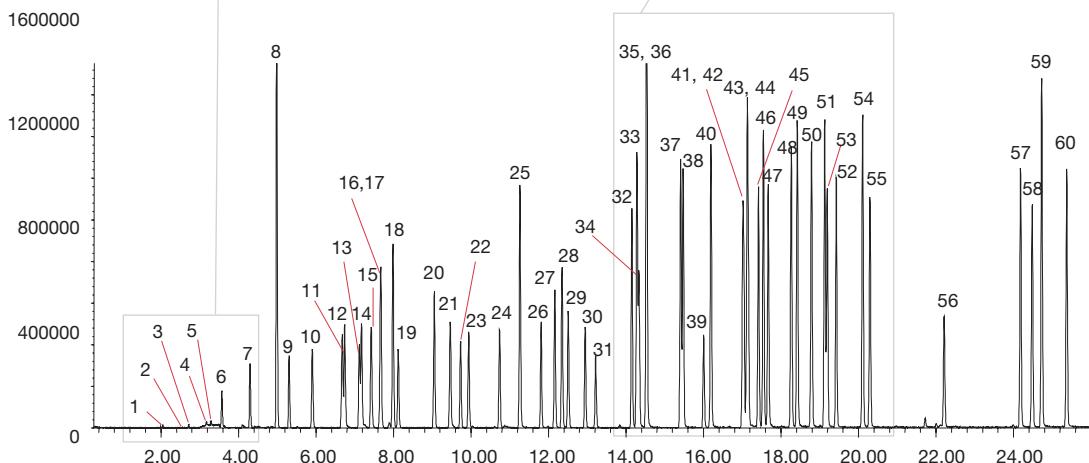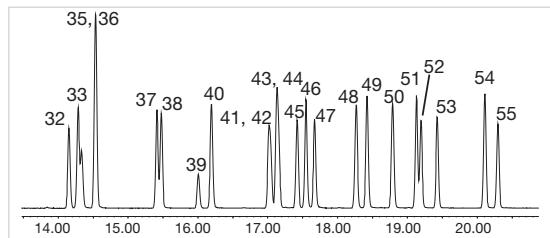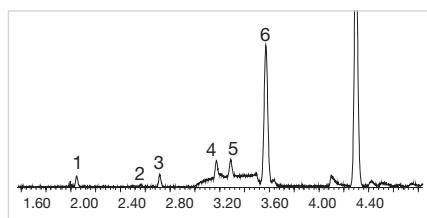

Notes. Chromatogram showing analysis of commonly screened volatile organic pollutants

## Components

- |                             |                                 |
|-----------------------------|---------------------------------|
| 1. Dichlorodifluoromethane  | 20. Trichloroethene             |
| 2. Chloromethane            | 21. 1,2-Dichloropropane         |
| 3. Vinyl chloride           | 22. Bromomethane                |
| 4. Bromomethane             | 23. Bromodichloromethane        |
| 5. Chloroethane             | 24. cis-1,3-Dichloropropene     |
| 6. Trichlorodifluoromethane | 25. Toluene                     |
| 7. 1,1-Dichloroethene       | 26. trans-1,3-Dichloropropene   |
| 8. Dichloromethane          | 27. 1,1,2-Trichloroethane       |
| 9. trans-1,2-Dichloroethene | 28. Tetrachloroethene           |
| 10. 1,1-Dichloroethane      | 29. 1,3-Dichloropropane         |
| 11. 2,2-Dichloropropane     | 30. Dibromochloromethane        |
| 12. cis-1,2-Dichloroethene  | 31. 1,2-Dibromoethane           |
| 13. Bromochloromethane      | 32. Chlorobenzene               |
| 14. Chloroform              | 33. Ethylbenzene                |
| 15. 1,1,1-Trichloroethane   | 34. 1,1,1-Tetrachloroethane     |
| 16. 1,1-Dichloropropene     | 35. p-Xylene                    |
| 17. Carbon tetrachloride    | 36. m-Xylene                    |
| 18. Benzene                 | 37. o-Xylene                    |
| 19. 1,2-Dichloroethane      | 38. Styrene                     |
|                             | 39. Bromoform                   |
|                             | 40. Isopropylbenzene            |
|                             | 41. Bromobenzene                |
|                             | 42. 1,1,2,2-Tetrachloroethane   |
|                             | 43. 1,2,3-Trichloropropane      |
|                             | 44. n-Propyl benzene            |
|                             | 45. 2-Chlorotoluene             |
|                             | 46. 1,3,5-Trimethylbenzene      |
|                             | 47. 4-Chlorotoluene             |
|                             | 48. tert-Butylbenzene           |
|                             | 49. 1,2,4-Trimethylbenzene      |
|                             | 50. sec-Butylbenzene            |
|                             | 51. 1,3-Dichlorobenzene         |
|                             | 52. p-Isopropyltoluene          |
|                             | 53. 1,2-Dichlorobenzene         |
|                             | 54. n-Butylbenzene              |
|                             | 55. 1,4-Dichlorobenzene         |
|                             | 56. 1,2-Dibromo-3-chloropropane |
|                             | 57. 1,2,4-Trichlorobenzene      |
|                             | 58. Hexachlorobutadiene         |
|                             | 59. Naphthalene                 |
|                             | 60. 1,2,3-Trichlorobenzene      |




GC Columns and Applications

## ENV 20 | Analysis of Polychlorinated p-Dibenzodioxins on BPX5


Column Part No.:	054114
Phase:	BPX5, 0.25 µm
Column:	50 m x 0.22 mm ID
Initial Temp.:	80 °C, 2 min
Rate 1:	4 °C/min
Temp 2:	220 °C
Rate 2:	5 °C/min

Temp. 3:	235 °C, 7 min
Rate 3:	5 °C/min
Final Temp.:	330 °C, 6 min
Detector:	High Resolution
Mass Spectrometer	He, 15 psi
Carrier Gas:	He, 300 psi
Injection Mode	Splitless, 270 °C


## Hexachlorodibenzodioxins

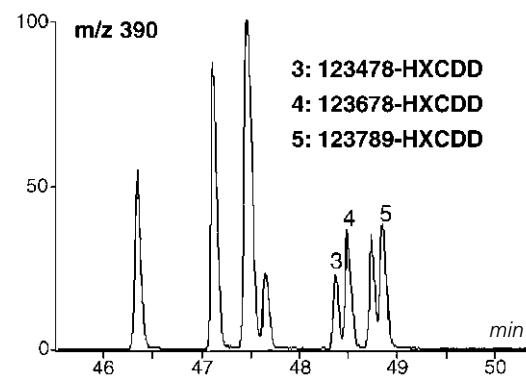


## Tetrachlorodibenzodioxins

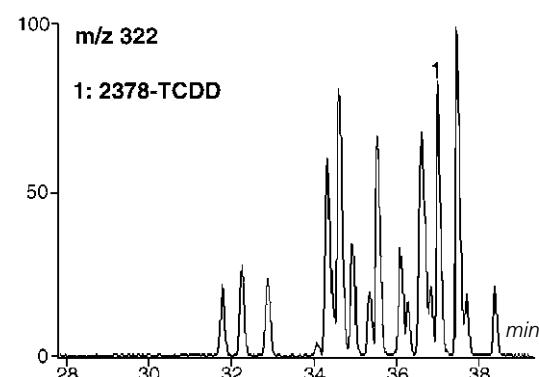


## Heptachlorodibenzodioxins

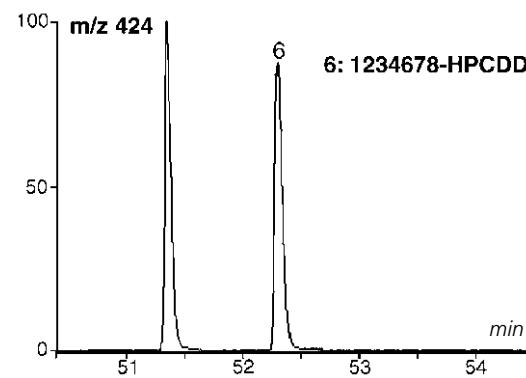


## Pentachlorodibenzodioxins

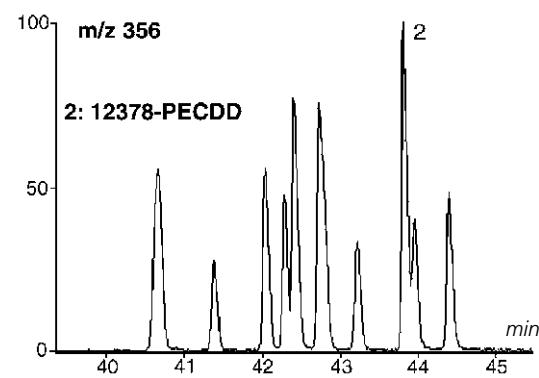

## Octachlorodibenzodioxin

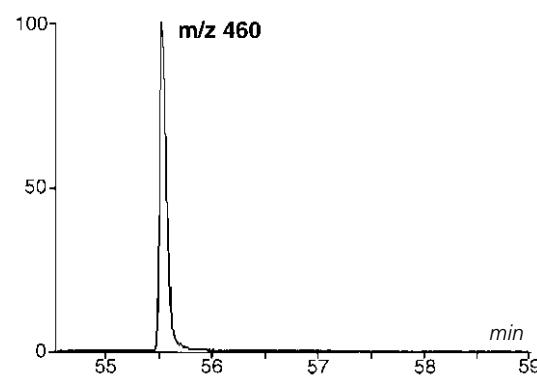

SGE wishes to acknowledge CARSO, 321 Avenue Jean Jaures,  
69362 LYON CEDEX 7, FRANCE

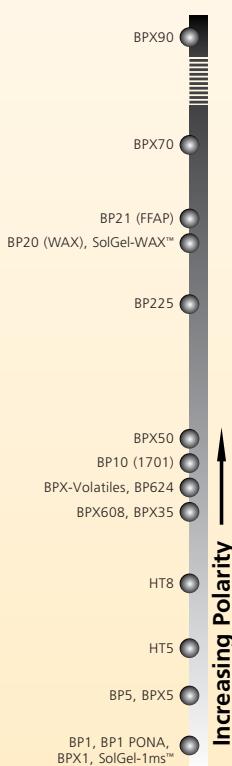


## ENV 57 | 8081 Organochlorine Pesticide Mix on BPX35



GC Columns and Applications

Column Part No.:	054701
Phase:	BPX35 0.25 µm film
Column:	30 m x 0.25 mm ID
8081 Standard:	10 ng/ µL in dichloromethane
Initial Temp.:	40 °C, 1 min.
Rate 1:	30 °C to 190 °C, 3 min
Rate 2:	10 °C to 300 °C
Final Temp.:	300 °C, 5 min.
Detector Type:	MSD
Carrier Gas:	He, 10.0 psi
Carrier Gas Flow:	1.3 mL/min
Constant Flow:	On
Average Linear Velocity:	36 cm/sec at 40 °C
Injection Mode:	Splitless
Purge on Time:	1 min.
Purge on (Split) Vent Flow:	60 mL/min.
Injection Volume:	1 µL
Injection Temp.:	250 °C
Autosampler:	No
Liner Type:	4 mm ID Double Taper Liner
Liner Part Number:	092018

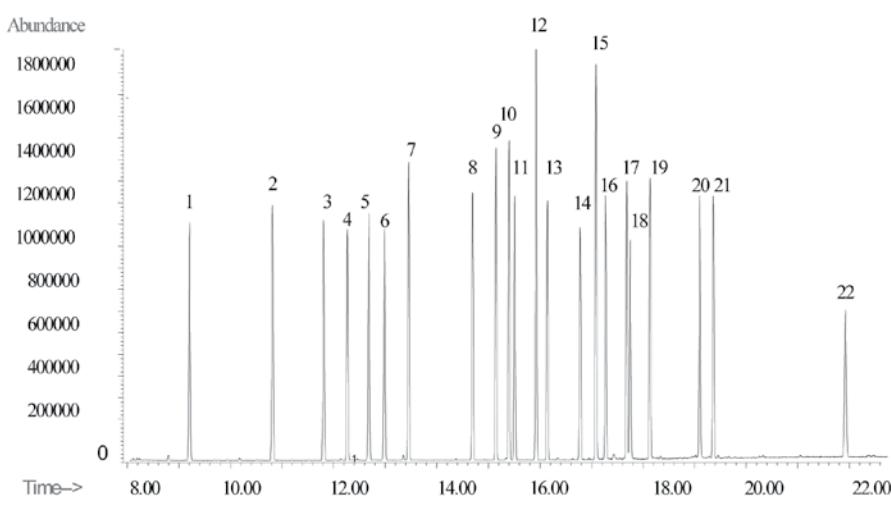

### Components

1. 2,4,5,6-tetrachloro-meta-xylene
2.  $\alpha$ -BHC
3.  $\gamma$ -BHC
4.  $\beta$ -BHC
5. Heptachlor
6.  $\delta$ -BHC
7. Aldrin
8. Heptachlorepoxy
9. trans-Chlordane
10. cis-Chlordane
11. Endosulfan A
12. DDE
13. Dieldrin
14. Endrin
15. DDD
16. Endosulfan B
17. DDT
18. Endrin Aldehyde
19. Endosulfan Sulfate
20. Methoxychlor
21. Endrin Ketone
22. Decachlorobiphenyl

## ENV 03 | Analysis of 18 Chlorinated Pesticides on BPX5


Part No.:	054125
Phase:	BPX5, 0.5 µm film
Column:	25 m x 0.32 mm ID
Initial Temp.:	170 °C
Rate:	7 °C
Final Temp.:	290 °C, 5 min
Detector:	ECD at 310 °C
Injection Mode:	Split
Carrier Gas:	He, 7 psi


Notes: Combined with the BPX608 column, BPX5 is the perfect confirmation column.

### Components

20ng/ µL each component

1.  $\alpha$ -BHC
2.  $\gamma$ -BHC
3.  $\beta$ -BHC
4. Heptachlor
5.  $\delta$ -BHC
6. Aldrin
7. Heptachlorepoxyde (isomer B)
8. Endosulfan I
9. 4,4'-DDE
10. Dieldrin
11. Endrin
12. 4,4'-DDD
13. Endosulfan II
14. 4,4'-DDT
15. Endrin aldehyde
16. Endosulfan sulfate
17. Methoxychlor
18. Endrin ketone

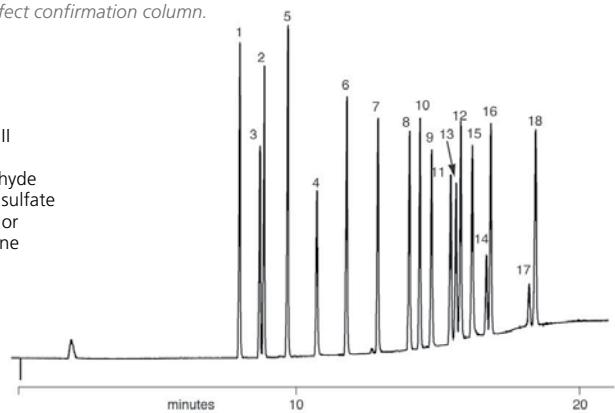


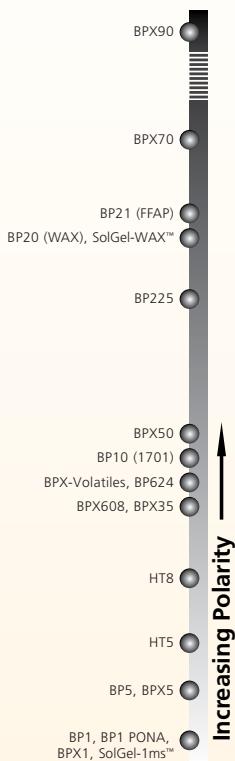

## ENV 59 | 8141 Organophosphorous Pesticide Mix on BPX5

Column Part No.:	054101
Phase:	BPX5 0.25 µm film
Column:	30 m x 0.25 mm ID
8141 Standard:	10 ng/µL in dichloromethane
Initial Temp.:	50 °C, 1 min
Rate 1:	30 °C/min to 190 °C, 3 min
Rate 2:	10 °C/min to 300 °C
Final Temp.:	300 °C, 5 min.
Detector Type:	MSD
Carrier Gas:	He, 11.1 psi
Carrier Gas Flow:	1.3 mL/min

Constant Flow:	On
Average Linear Velocity:	42 cm/sec at 50 °C
Injection Mode:	Splitless
Purge on Time:	0.5 min
Purge on (Split) Vent Flow:	60 mL/min
Injection Volume:	1 µL
Injection Temperature:	250 °C
Autosampler:	No
Liner Type:	4 mm ID Double Taper Liner
Liner Part Number:	092018

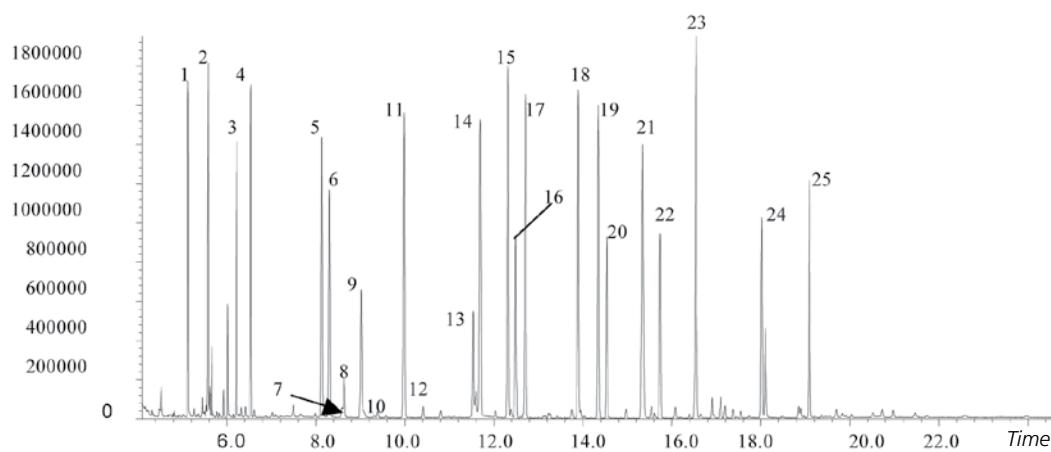**Components**

- |                                     |                      |                        |
|-------------------------------------|----------------------|------------------------|
| 1. 4-Chloro-3-nitrobenzotrifluoride | 8. Naled             | 17. Trichlorinate      |
| 2. Dichlorvos                       | 9. Phorate           | 18. Tetrachlorvinphos  |
| 3. 1-Bromo-2-nitrobenzene           | 10. Demeton          | 19. Tokuthion          |
| 4. α-Mevinphos                      | 11. Diazinon         | 20. Impurity           |
| 5. Tri-butylphosphate               | 12. Disulfoton       | 21. Fensulfothion      |
| 6. Ethoprop                         | 13. Methyl parathion | 22. Impurity           |
| 7. Sulfotep                         | 14. Ronnel           | 23. Triphenylphosphate |
|                                     | 15. Chloryrifos      | 24. Guthion            |
|                                     | 16. Fenthion         | 25. Coumaphos          |

## ENV 45 | Organophosphorous Pesticides on BPX50




GC Columns and Applications

Column Part No.:	<b>054751</b>	Column Part Number:	<b>054740</b>
Phase:	BPX50, 0.25 µm film	Phase:	BPX50, 0.10 µm film
Mixture of:	10 ng/ µL	Mixture of 10 ng/ µL	42 cm/sec at 50 °C
Organophosphorous Pesticides:	10 ng/ µL in	Organophosphorous Pesticides	Splitless
Column:	30 m x 0.25 mm ID	Column:	10 m x 0.10 mm ID
Initial Temp:	50 °C , 1 min	Initial Temp.:	70 °C , 1 min
Rate 1:	30 °C/min to 200 °C, 3 min	Rate 1:	25 °C/min to 320 °C
Rate 2:	10 °C/min to 310 °C	Rate 2:	N/A
Final Temp:	310 °C, 2 min	Final Temp:	320 °C, 0 min
Detector Type:	FID, 320 °C	Detector Type:	FID, 320 °C
Carrier Gas:	He, 14.4 psi	Carrier Gas:	He, 39.0 psi
Carrier Gas Flow:	1.30 mL/min	Carrier Gas Flow :	0.370 mL/min
Constant Flow:	On	Constant Flow:	On
Average Linear Velocity:	30 cm/sec at 50 °C	Average Linear Velocity:	35 cm/sec at 70 °C
Injection Mode:	Splitless	Injection Mode:	Split
Purge On Time:	0.5 min	Purge On Time:	1.0
Purge On (Split) Vent Flow:	60 mL/min	Purge On (Split) Vent Flow:	10 mL/min
Injection Volume:	1.0 µL	Injection Volume:	0.5 µL
Injection Temperature:	240 °C	Injection Temperature:	240 °C
Autosampler:	Yes	Autosampler:	Yes
Liner Type:	4 mm ID FocusLiner™ with single taper	Liner Type :	2.3 mm ID FocusLiner™
Liner Part Number:	092003	Liner Part Number:	092005


### NORMAL

Chromatogram showing separation of Organophosphous Pesticides using a conventional 30 meter x 0.25 mm ID BPX50 column with a 0.25 micron film.

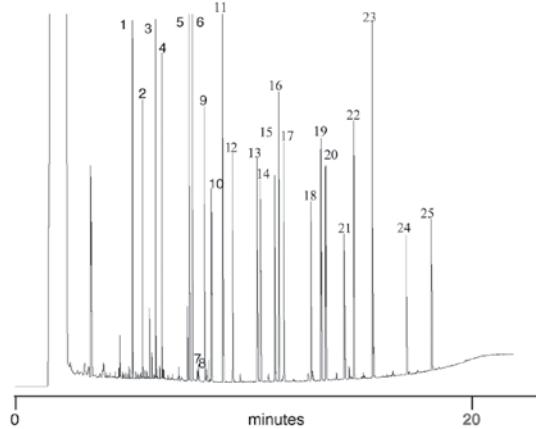

### FAST

Chromatogram showing separation of Organophosphous Pesticides using a **FAST** BPX50 column.

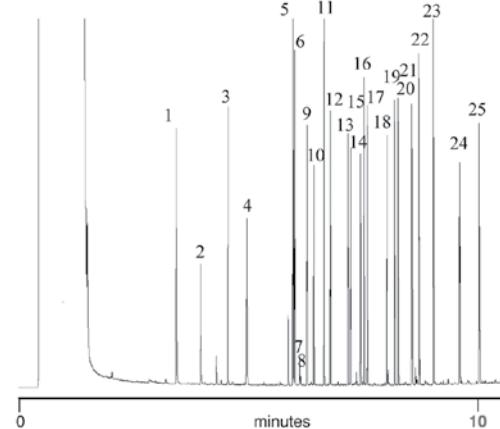

#### Components

- |                                      |                             |
|--------------------------------------|-----------------------------|
| 1. 4-Chloro-3-nitrobenzo-trifluoride | 8. Naled                    |
| 2. Dichlorvos                        | 9. Phorate                  |
| 3. 1-Bromo-2-nitrobenzene            | 10. Demeton                 |
| 4. $\alpha$ -Mervinphos              | 11. Diazinon                |
| 5. Tributylphosphate (IS)            | 12. Disulfoton              |
| 6. Ethoprop                          | 13. Methyl Parathion        |
| 7. Sulfotep                          | 14. Ronnel                  |
|                                      | 15. Chlorpyrifos            |
|                                      | 16. Fenthion                |
|                                      | 17. Trichlorinate           |
|                                      | 18. Tetrachlorvinphos       |
|                                      | 19. Tokuthion               |
|                                      | 20. Impurity                |
|                                      | 21. Fensulfothion           |
|                                      | 22. Impurity                |
|                                      | 23. Triphenylphosphate (IS) |
|                                      | 24. Guthion                 |
|                                      | 25. Coumaphos               |




GC Columns and Applications

## ENV 04 | Analysis of Herbicides on BPX35


Column Part No.:	054711	Final Temp.:	300 °C 5 min
Phase:	BPX35, 0.25 µm film	Detector:	FID, 380 °C
Column:	25 m x 0.22 mm ID	Injection Mode:	Split (20:1)
Initial Temp.:	80 °C	Carrier Gas:	He, 100 kpa
Rate:	10 °C/min		

Note: BPX35 provides quick analysis of all 3 Triazine compounds

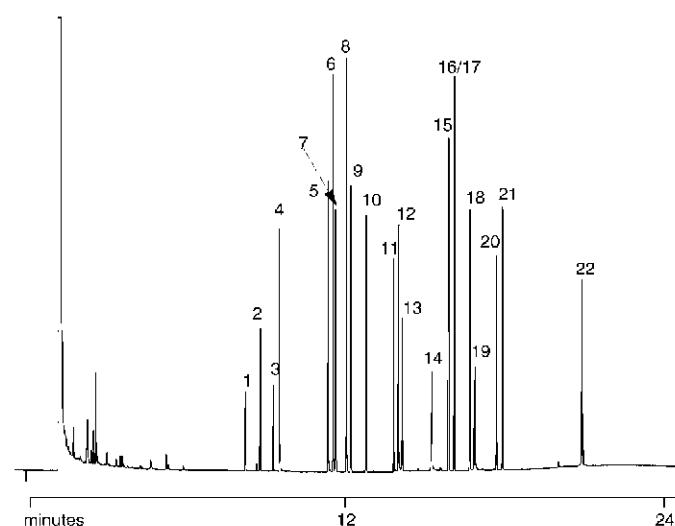
**Components**

1. Eptam®
2. Sutan®
3. Vernam®
4. Tillam®
5. Ordram®
6. Treflan®
7. Balan®
8. Ro-Neet®
9. Propachlor
10. Tolban®
11. Propazine
12. Atrazine
13. Simazine
14. Terbacil
15. Sencor®
16. Dual®
17. Paarlan®
18. Prowl®
19. Bromacil
20. Oxadiazon
21. GOAL®
22. Hexazinone

## ENV 48 | Analysis of Herbicides on BPX5

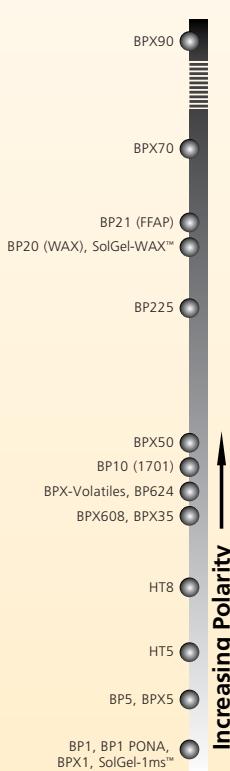

Column Part No.:	054101	Rate 2:	5 °C/min
Phase:	BPX5, 0.25 µm	Final Temp.:	260 °C, 10 min
Column:	30 m x 0.25 mm ID	Detector:	NPD
Initial Temp.:	90 °C, 1 min	Injection Mode:	Varian SPI
Rate 1:	30 °C/min	Carrier Gas:	He, 10 psi
Temp.:	180 °C		

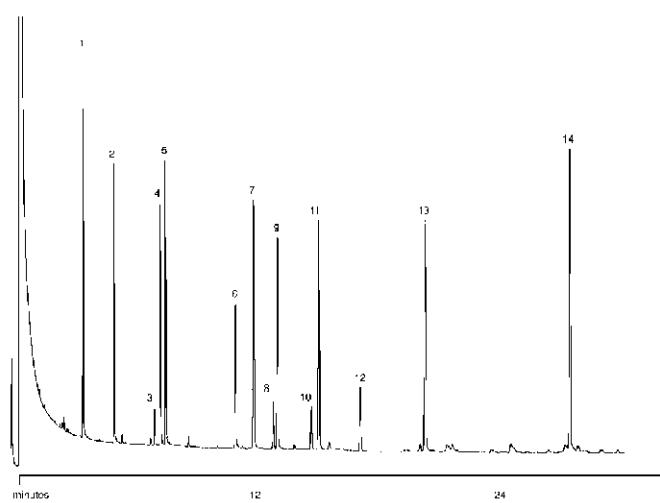**Components**


1. Metamidofos
2. Acephate
3. Diphenylamine
4. Monocrotophos
5. Sulfotep
6. Tolclofos-methyl
7. Fenitrothion
8. Triadimefon
9. Trichloronate
10. Triadimenol
11. Bromophos-ethyl
12. Bupirimate
13. Carbophenothion
14. Dialifos

## ARO 14 | Analysis of chlorinated and nitroaromatic compounds on SolGel-1ms™



GC Columns and Applications

Column Part No.:	054462
Phase:	SolGel-1ms™ 0.25 µm film
Sample:	200 ppm in dichloromethane
Column:	30 m x 0.25 mm ID
Initial Temp:	40 °C, 1 min.
Rate 1:	10 °C/min to 300 °C
Final Temp:	300 °C, 2 min.
Detector Type:	MSD
Carrier Gas:	He, 25.7 psi
Carrier Gas Flow:	1.8 mL/min.
Constant Flow:	On
Average Linear Velocity:	35 cm/sec, 40 °C
Injection Mode:	Split
Split Ratio:	100 : 1
Injection Volume:	0.5 µL
Injection Tem:	250 °C
Liner Type:	4 mm ID Single Taper Liner
Liner Part No.:	092017
Full Scan / SIM:	Full scan 45-450

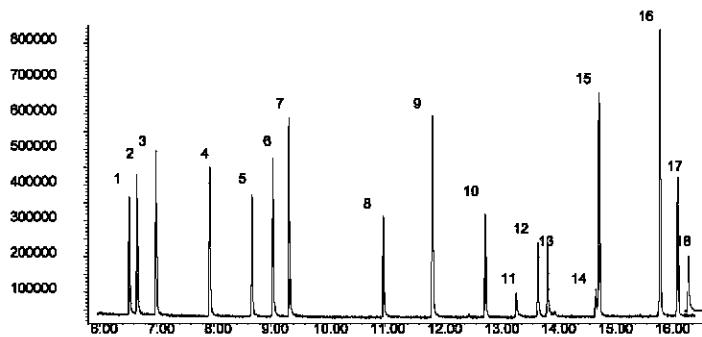


### Components

1. Phenol
2. o-Chlorophenol
3. p-Dichlorobenzene
4. Nitrobenzene
5. o-Nitrophenol
6. 2,4-Xylenol
7. 2,4-Dichlorophenol
8. 4-Chloro-3-methylphenol
9. 2,4,6-Trichlorophenol
10. 2,6-Dinitrotoluene
11. 2,4-Dinitrophenol
12. 2,4-Dinitrotoluene
13. 4-Nitrophenol
14. 4,6-Dinitro-o-cresol
15. 4-Chlorophenyl phenyl ether
16. 4-Bromophenyl phenyl ether
17. Hexachlorobenzene
18. Pentachlorophenol

## ALC 06 | US EPA 625 Phenols Mix on BPX50

Column Part No.:	054751
Phase:	BPX50, 0.25 µm
Column:	30 m x 0.25 mm ID
Injector Mode:	Split, 40:1
Initial Oven Temp:	50 °C, 1 min
Rate 1:	8 °C/min
Final Temp:	300 °C, 10 min
Detector:	HP 5973 MSD

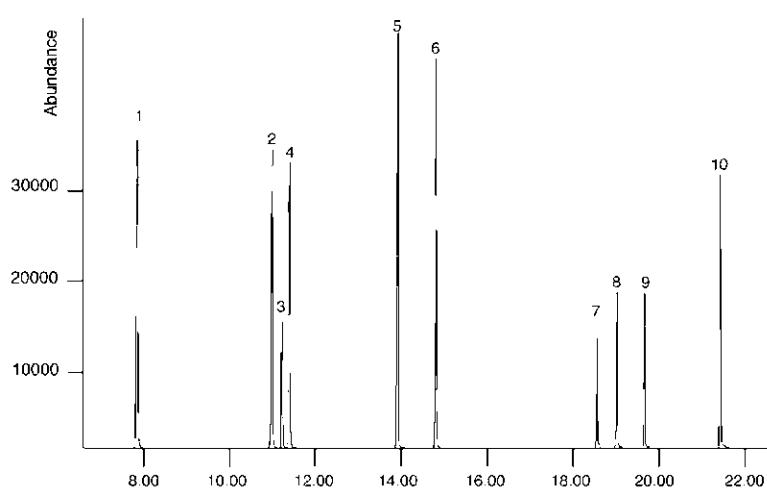

### Components

1. 2-Chlorophenol
2. 2-Nitrophenol
3. 2, 4-Dimethylphenol
4. 2, 4-Dichlorophenol
5. 4-Chloro-3-methylphenol
6. 2, 4, 6-Trichlorophenol
7. 2, 4-Dinitrophenol
8. 4-Nitrophenol
9. 2-Methyl-4, 6-dinitrophenol
10. Pentachlorophenol




GC Columns and Applications

## ENV 65 | Analysis of Synthetic Pyrethroids on BPX50

Column Part No.:	054751
Phase:	BPX50, 0.25 µm film
Column:	30 m x 0.25 mm ID 16
Pyrethroids:	10 ppm in methanol
Initial Temp.:	50 °C, 1 min.
Rate 1:	30 °C/min to 200 °C
Rate 2:	4 °C/min to 300 °C
Final Temp.:	300 °C, 5 min
Detector Type:	MSD
Carrier Gas:	He, 6.8 psi
Carrier Gas Flow:	1.0 mL/min

Constant Flow:	On
Average Linear Velocity:	36 cm/sec at 50 °C
Injection Mode:	Splitless
Purge on Time:	0.5 min
Purge on (Split) Vent Flow:	60 mL/min
Injection Volume:	1 µL
Injection Temperature:	250 °C
Autosampler:	No
Liner Type:	4 mm ID Double Taper Liner
Liner Part Number:	092018

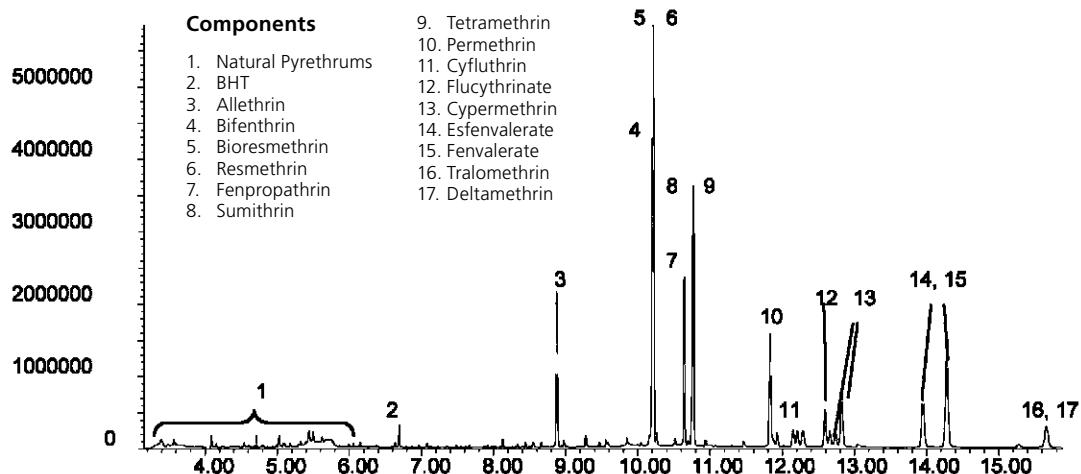


## ARO 13 | Analysis of BTEX on SolGel-WAX™

Column Part No.:	054796
Phase:	SolGel-WAX™ 0.25 µm film
BTEX:	300 ppm in methanol
Column:	30 m x 0.25 mm ID
Initial Temp.:	60 °C, 10 min
Detector Type:	FID
Carrier Gas:	He, 17.3 psi
Carrier Gas Flow:	1.5 mL/min

Constant Flow:	On
Average Linear Velocity:	35 cm/sec, 60 °C
Injection Mode:	Split
Split Ratio:	100:1
Injection Volume:	0.2 µL
Injection Temp.:	250 °C
Liner Type:	4 mm ID Double Taper Line
Liner Part Number:	092018

Increasing Polarity ↑

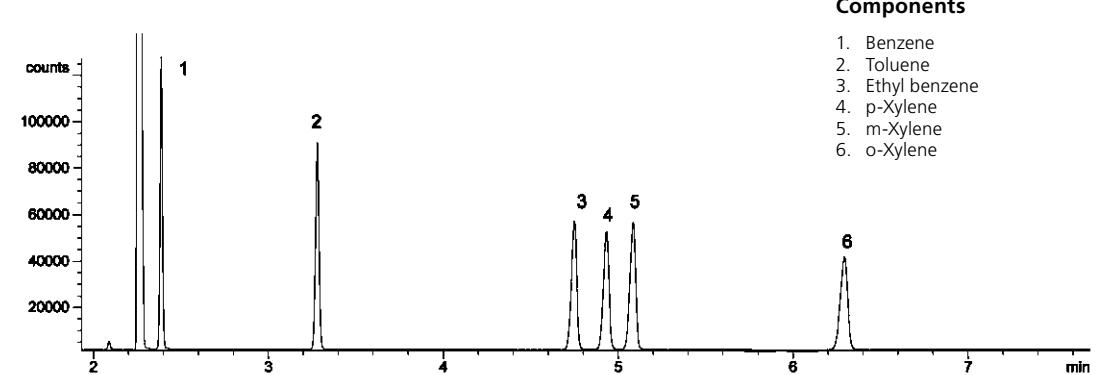


## ENV 84 | Analysis of US EPA 8270 Mix on BPX5



GC Columns and Applications

Column Part No.:	054101
Phase:	BPX5, 0.25 µm film
Column:	30 m x 0.25 mm
ID Sample:	5 ppm solution
Initial Temp.:	40 °C, 3 min
Rate 1:	8 °C/min to 300 °C
Final Temp.:	300 °C, 9 min.
Detector Type:	Mass Spectrometer
Carrier Gas:	He
Inlet Pressure:	16 psi for 30 sec then drops to 10 psi
Pressure rate1:	10 psi to 28 psi at 0.5 psi/min
Final Pressure:	28 psi until end of run
Carrier Gas Flow:	1.1 mL/min.
Constant Flow:	On
Injection Mode:	Splitless
Purge on Time:	0.5 min
Purge on (Split) Vent Flow:	40 mL/min
Injection Volume:	1 µL
Injection Temperature:	250 °C
Autosampler:	No
Liner Type:	4 mm ID Single Gooseneck
Liner Part Number:	092017
Full Scan / SIM:	Full scan 41-450

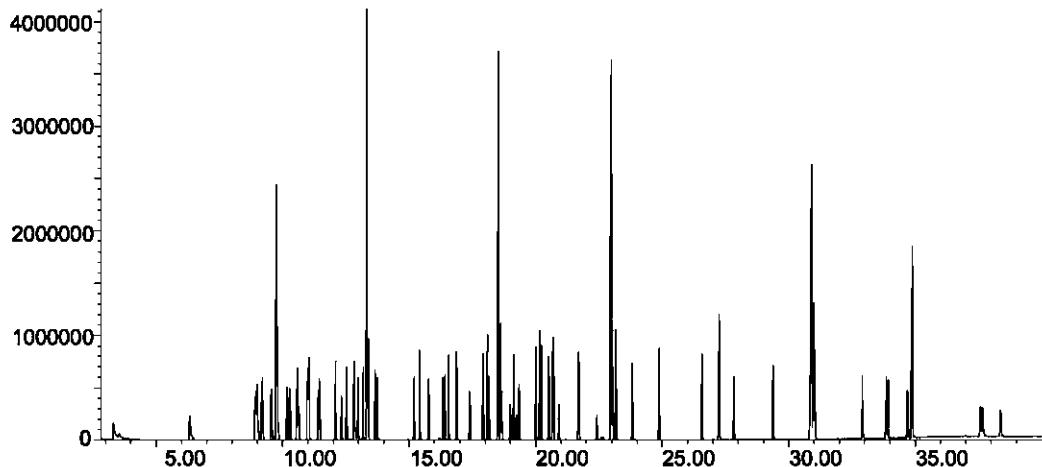





### Components

1. Pyridine
2. n-Nitrosodimethylamine
3. 2-Fluorophenol
4. Phenol-d5
5. Phenol
6. Aniline
7. 2-Chlorophenol
8. bis-(2-chloroethyl) ether
9. 1,3-Dichlorobenzene
10. 1,4-Dichlorobenzene-d4
11. 1,4-Dichlorobenzene
12. 1,2-Dichlorobenzene
13. Benzyl alcohol
14. 2-Methyl phenol
15. bis-(2-chloroisopropyl)ether
16. n-Nitroso-di-n-propylamine
17. Hexachloroethane
18. 4-Methylphenol
19. Nitrobenzene-d5
20. Nitrobenzene
21. Isophorone
22. 2-Nitrophenol
23. 2,4-Xylenol
24. bis- (2-Chloroethoxy) methane
25. Benzoic acid
26. 2,4-Dichlorophenol
27. 1,2,4-Trichlorobenzene
28. Naphthalene-d8
29. Naphthalene
30. Hexachlorobutadiene
31. 4-Chloroaniline
32. 4-Chloro-3-methylphenol
33. 2-Methylnaphthalene
34. Hexachlorocyclopentadiene
35. 2,4,6-Trichlorophenol
36. 2,4,5-Trichlorophenol
37. 2-Fluorobiphenyl
38. 2-Chloronaphthalene
39. 2-Nitroaniline
40. Dimethyl phthalate
41. Acenaphthylene
42. 2,6-Dinitrotoluene
43. Acenaphthene-d10
44. Acenaphthene
45. 3-Nitroaniline
46. 2,4-Dinitrophenol
47. Dibenzofuran
48. 4-Nitrophenol
49. 2,4-Dinitrotoluene
50. Diethylphthalate
51. Fluorene
52. 4-Chlorophenyl phenyl ether
53. 2-Methyl-4,6-dinitrophenol
54. 4-Nitroaniline
55. n-Nitrosodiphenylamine
56. Azobenzene
57. 2,4,6-Tribromophenol
58. 4-Bromophenyl phenyl ether
59. Hexachlorobenzene
60. Pentachlorophenol
61. Phenanthrene-d10
62. Phenanthrene
63. Anthracene
64. Carbazole
65. Di-n-butyl phthalate
66. Fluoranthene
67. Benzidine
68. Pyrene
69. p-Terphenyl-d14
70. Butyl benzyl phthalate
71. Benz[a]anthracene
72. Chrysene-d12
73. Chrysene
74. 3,3-Dichlorobenzidine
75. bis (2-Ethylhexyl) phthalate
76. Di-n-octyl phthalate
77. Benzo (b) fluoranthene
78. Benzo (k) fluoranthene
79. Benzo (a) pyrene
80. Perylene-d12
81. Indeno (1,2,3-cd) perylene
82. Dibenz (a,h) anthracene
83. Benzo[g,h,i]perylene



GC Columns and Applications

## ENV 84 continued

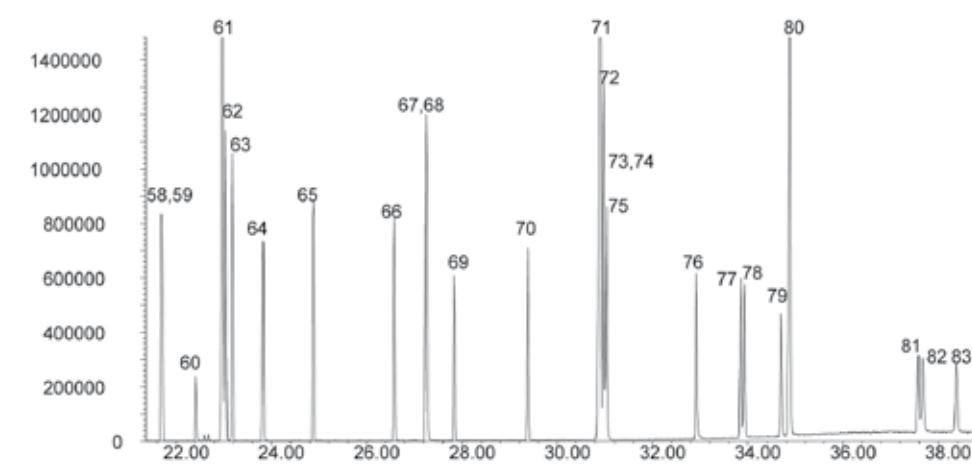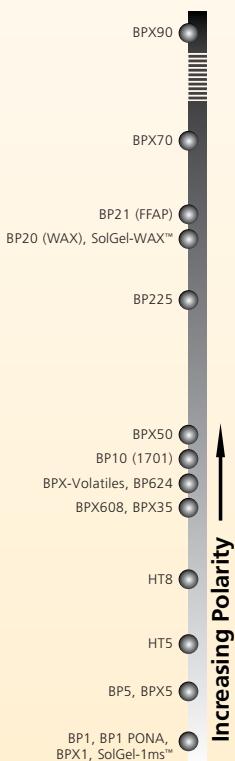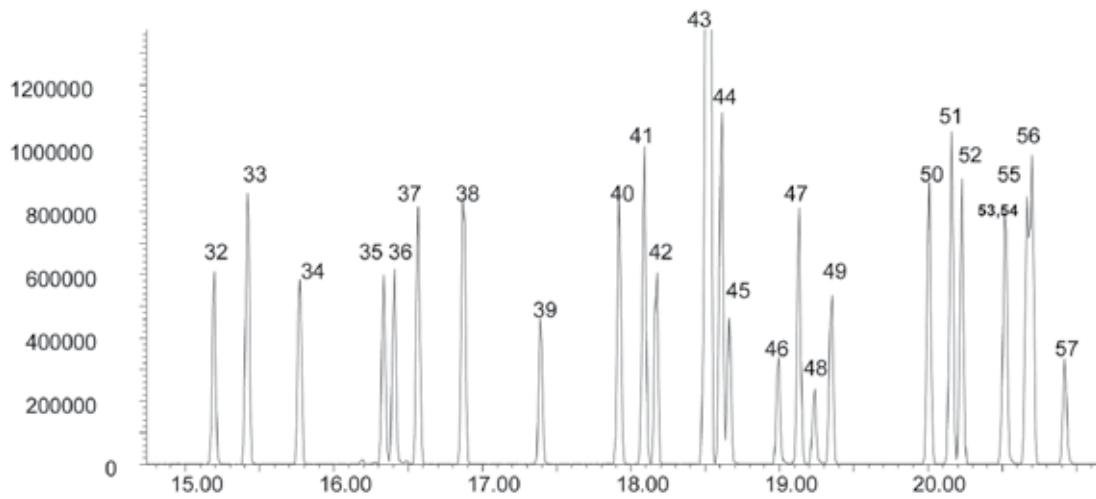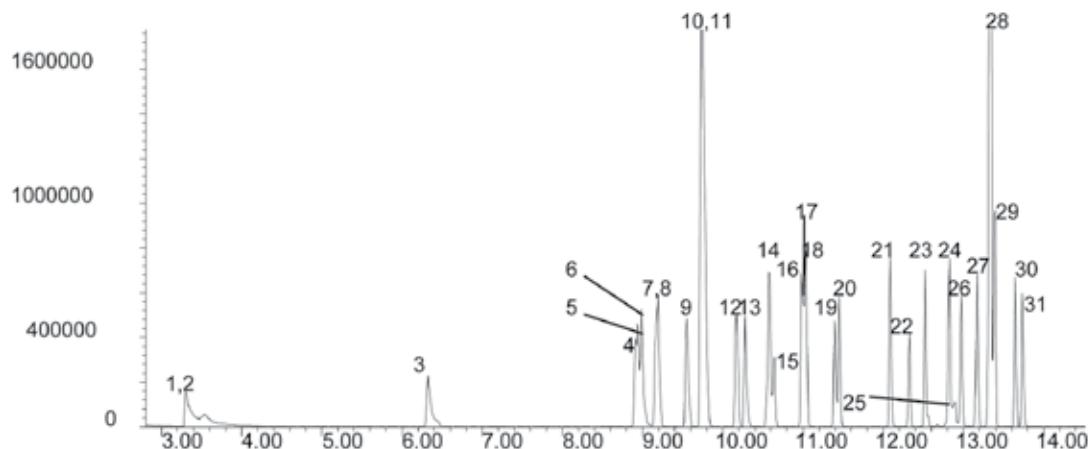

SGE would like to thank Mark Ferry from ECS/MDL USA for supplying all of the chromatograms for this application note.


GC Application by Industry | Food, Flavor, Fragrance

FOO 03 | Analysis of Scotch Whisky on BP20

<b>Column Part No.:</b>	<b>054447</b>
Phase:	BP20, 1.0 µm film
Column:	12 m x 0.53 mm ID
Initial Temp:	55 °C, 3 min
Rate:	10 °C/min
Final Temp:	120 °C, 0 min
Detector:	FID
Sensitivity:	128 x 10-12 AFS
Injection Mode:	Split

## Components

1. Acetaldehyde
  2. Ethyl Acetate
  3. Methanol
  4. Ethanol
  5. Propan-1-ol
  6. 2-Methylpropan-1-ol
  7. 2-Methylbutan-1-ol + 3-Methylbutan-1-ol

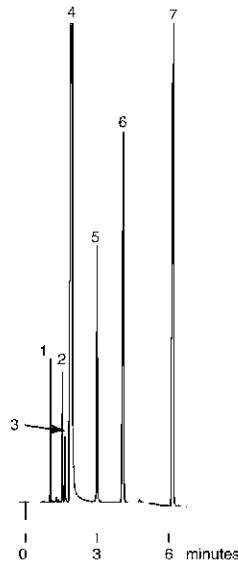


## GC Columns and Applications

AN-0022-C | FAME Analysis with BPX90 – A Highly Polar Column

<b>Column Part No.:</b>	<b>054570</b>
Phase:	90% Cyanopropyl Polysilphenylsiloxane
Column Dimensions:	15 m x 0.25 mm x 0.25 µm
Injector Temperature:	250 °C
Injection Volume:	1.0 µL
Injector Type:	Split
Split Ratio:	100:1
Liner Type:	FocusLiner™
Carrier Gas:	Helium

Constant Flow:	ON
Pressure:	4.02 psi
Column Flow Rate:	1.3 ml/min
Linear Velocity:	59 cm/sec
Initial Temp.:	70 °C hold for 1 minute
Rate:	20 °C/min to 150 °C
Rate:	10 °C/min
Final Temp.:	250 °C hold for 5 minutes
Detector Type:	MSD

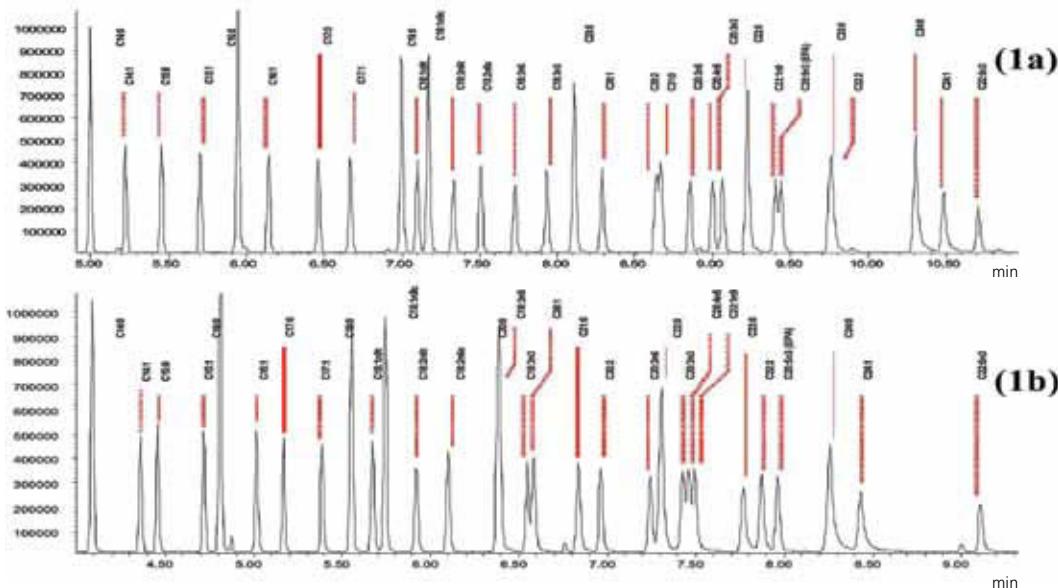

Supelco 37 FAME standard analyzed with (a) BPX70 and (b) BPX90

*SGE would like to thank J. Harynuk, P.J. Marriott and P. Wynne, Chromatographia, 2006; 63 (Supplement 13): S61-S66.*






GC Columns and Applications

## AN-0011-C | Analysis of Omega-3 Fatty Acids using a Highly Selective GC Capillary Column

Column Part No.:	054606
Phase:	BPX70, 0.25 µm film
Sample:	10 ppm in methanol
Column:	25 m x 0.32 mm ID
Initial Temp.:	80 °C, 2 min
Rate 1:	50 °C/min to 130 °C, 10 min
Rate 2:	2 °C/min to 172 °C
Final Temp.:	172 °C, 6 min
Detector Type:	FID
Detector Temp.:	300 °C
Carrier Gas:	He, 10 psi

Carrier Gas Flow:	2.2 mL/min
Constant Flow:	On
Average Linear Velocity:	39 cm/sec at 80 °C
Injection Mode:	Split
Split Ratio:	58:1
Injection Volume:	1 µL
Injection Temperature:	250 °C
Autosampler:	No
Liner Type:	4 mm ID FocusLiner™
Liner Part No.:	092002

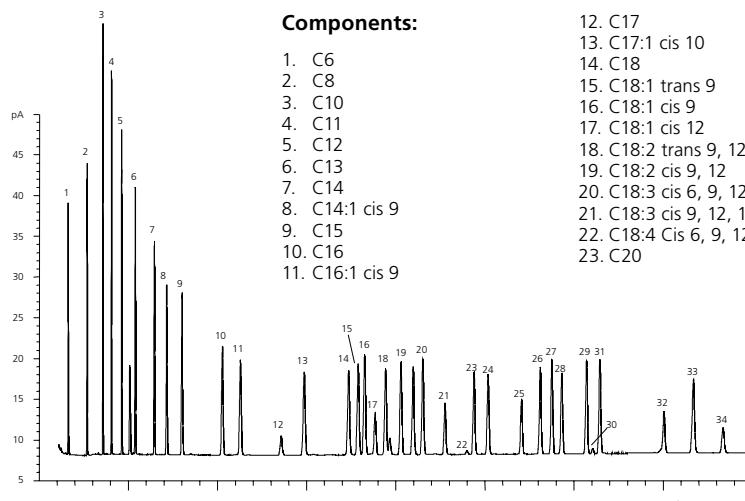


Notes: The chromatogram shows the excellent separation of a complex mixture of FAME compounds. Note the excellent peak shape and separation of the Omega-1,2 and 3 fatty acid isomers both structural and cis and trans.

SGE would like to thank Masterfoods UK for supplying the sample and chromatographic conditions for this chromatogram.

## FOO 16 | Analysis of Triglyceride Standards on HT5

Column Part No.:	054661
Phase:	HT5, 0.1 µm
Column:	6 m x 0.53 mm I.D. (Aluminum Clad)
Initial Temp.:	60 °C, 0 min
Program Rate:	10 °C/min
Final Temp.:	370 °C, 5 min
Carrier Gas:	H <sub>2</sub> , 2 psi
Detector:	F.I.D.
Sensitivity:	32 x 10-12 AFS
Injection Mode:	On-column

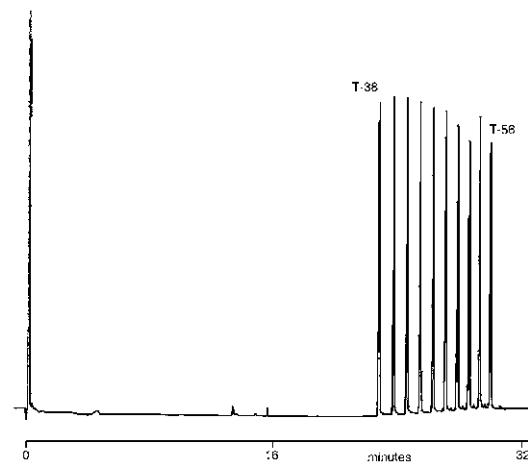


Notes: For the analysis of triglycerides, on-column injection is recommended. Temperatures above 380 °C are not recommended as triglycerides can degrade.

BPX90  
BPX70  
BP21 (FFAP)  
BP20 (WAX), SolGel-WAX™  
BP225  
BPX50  
BP10 (1701)  
BPX-Volatiles, BP624  
BPX608, BPX35  
HT8  
HT5  
BP5, BPX5  
BP1, BP1 PONA,  
BPX1, SolGel-1ms™

Increasing Polarity ↑

## FLA 05 | Analysis of Menthol Oil on CYDEX-B


<b>Column Part No.:</b>	<b>054901</b>	Final Temp.:	130 °C
Phase:	Cydex-B, 0.25 µm film	Carrier Gas:	H <sub>2</sub>
Column:	50 m x 0.22 mm I.D.	Detector:	F.I.D.
Initial Temp.:	100 °C, 5 min	Sensitivity:	32 x 10-12 AFS
Rate:	2 °C/min	Injection Mode:	Split

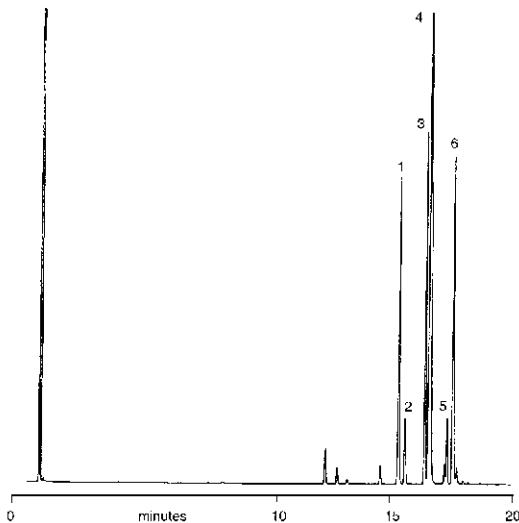

Notes: Cydex - B column enables the separation of three different enantiomer pairs in Menthol Oil.

## FLA 19 | Analysis of Eucalyptus Oil on SolGel-WAX™

<b>Column Part No.:</b>	<b>054796</b>	Constant Flow:	On
Phase:	SolGel-WAX™, 0.25 µm film	Average Linear Velocity:	35 cm/sec at 40 °C
Sample:	Neat	Injection Mode:	Split
Column:	30 m x 0.25 mm ID	Split Ratio:	100:1
Initial Temp.:	40 °C, 1 min.	Injection Volume:	0.2 µL
Rate 1:	8 °C/min to 220 °C,	Injection Temp.:	250 °C
Final Temp.:	220 °C, 5 min.	Liner Type:	4 mm ID Single Taper Liner
Detector Type:	Mass Spectrometer	Liner Part Number:	092017
Carrier Gas:	He, 25.7 psi	Full Scan / SIM:	Full scan 45-450
Carrier Gas Flow:	1.8 mL/min.		

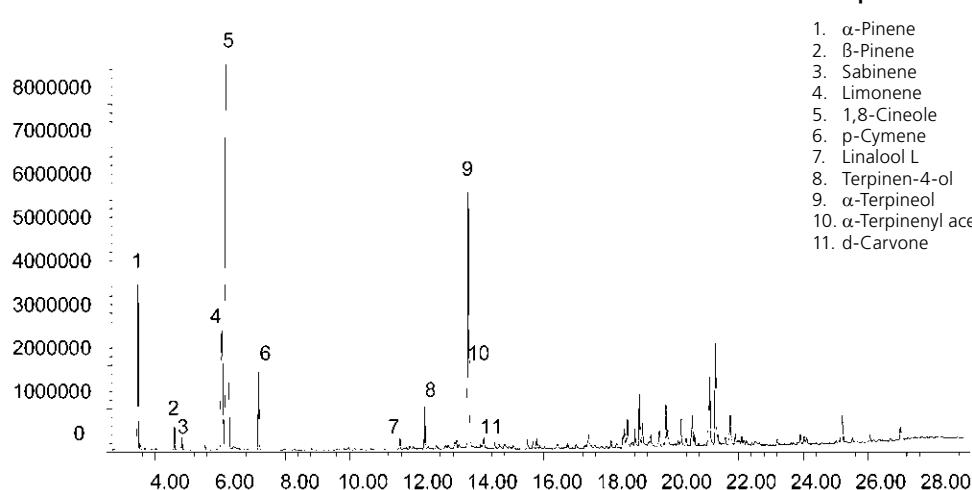

### Components


1. (+) Neomenthol
2. (-) Neomenthol
3. (+) Menthol
4. (-) Menthol
5. (+) α-Terpineol
6. (-) α-Terpineol

GC Columns and Applications



GC Columns and Applications

## FOO 02 | Analysis of Food Additives Antimicrobials on BP5

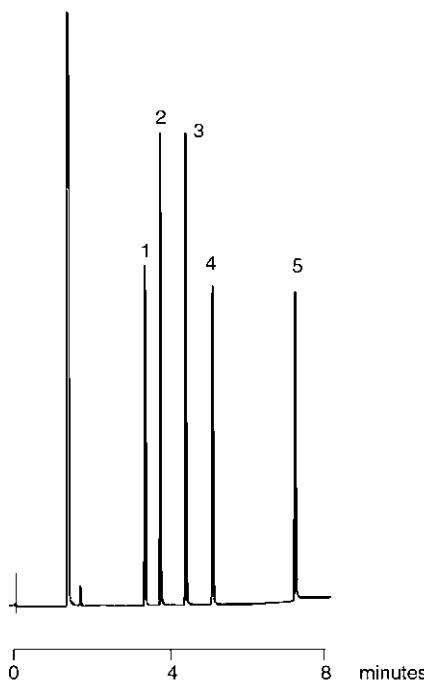

Column Part No.:	<b>054186</b>
Phase:	BP5, 0.5 µm film
Column:	25 m x 0.32 mm ID
Initial Temp:	160 °C, 0 min
Rate:	15 °C/min
Final Temp:	280 °C, 0 min
Detector:	FID
Sensitivity:	256 x 10-12 AFS
Injection Mode:	Split

**Components**

1. Methyl Paraben
2. Ethyl Paraben
3. Propyl Paraben
4. Butyl Paraben
5. Heptyl Paraben



## FOO 04 | Analysis Of 13 Sugar Component Alditol Acetate Mixture on BPX70

**Column Part No.:** **054622**

Phase:	BPX70, 0.25 µm film
Column:	30 m x 0.25 mm I.D.
Initial Temp.:	190 °C, 1 min.
Program Rate:	3 °C/min.
Final Temp.:	260 °C, 10min.
Carrier Gas:	He, 50 kPa
Detector:	MS (Electron Impact Ionisation, Ionisation Potential 70 eV) Scan 100 m/z to 350 m/z in 0.3 s.
Injection Mode:	Split 50:1

**Components**

1. Erythritol
2. 2-Deoxy-ribitol
3. Rhamnitol
4. Fucitol
5. Ribitol
6. Arabinitol
7. Xylitol
8. 2-Deoxy-glucitol
9. Allitol
10. Mannitol
11. Galactitol
12. Glucitol
13. Myo-inositol

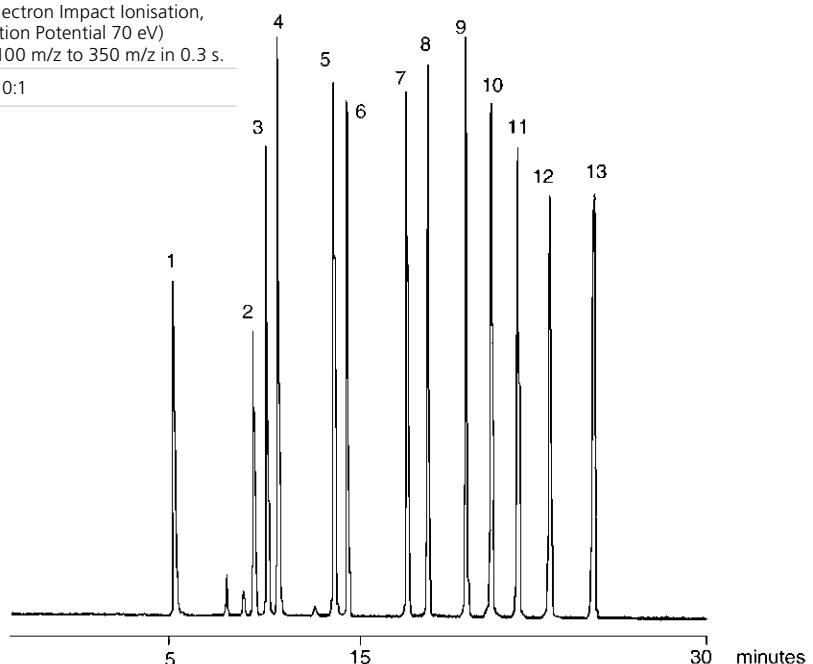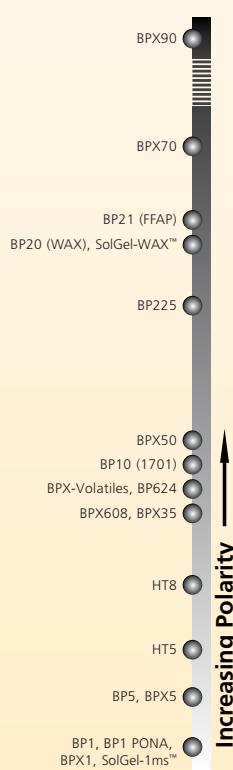

## FOO 21 | Plant Sterols




GC Columns and Applications

Column Part No.:	054148
Phase:	BPX5, 1.0 $\mu\text{m}$
Column:	30 m x 0.53 mm ID
Initial Temp.:	320 °C
Detector:	FID, 360 °C
Injector Mode:	split 100:1
Carrier Gas:	He, 3 psi
Injection Volume:	1 $\mu\text{L}$

### Components

- |                   |                     |
|-------------------|---------------------|
| 1. Coprostanol    | 7. Campasterol      |
| 2. Cholesterol    | 8. Stigmasterol     |
| 3. Cholestanol    | 9. Unknown          |
| 4. Desmosterol    | 10. beta-Sitosterol |
| 5. Brassicasterol | 11. Lanosterol      |
| 6. Ergosterol     |                     |

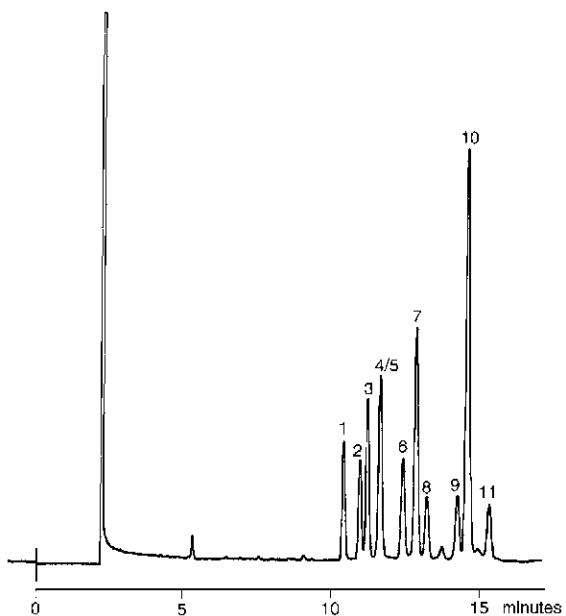


## FOO 24 | Analysis of Wine on BP20

Column Part No.:	054442
Phase:	BP20, 1.0 $\mu\text{m}$
Column:	25 m x 0.32 mm ID
Initial Temp.:	40 °C, 2 min
Rate 1:	5 °C/min
Temp 2:	50 °C
Rate 2:	15 °C/min
Final Temp.:	190 °C
Carrier Gas:	H <sub>2</sub> , 6 psi
Injection Mode:	2 $\mu\text{L}$

### Components

- |                  |                    |
|------------------|--------------------|
| 1. Acetaldehyde  | 6. Propanol        |
| 2. Ethyl Acetate | 7. Isobutanol      |
| 3. Methanol      | 8. Isoamyl Alcohol |
| 4. Isopropanol   | 9. Acetic Acid     |
| 5. Ethanol       | 10. Unknown        |

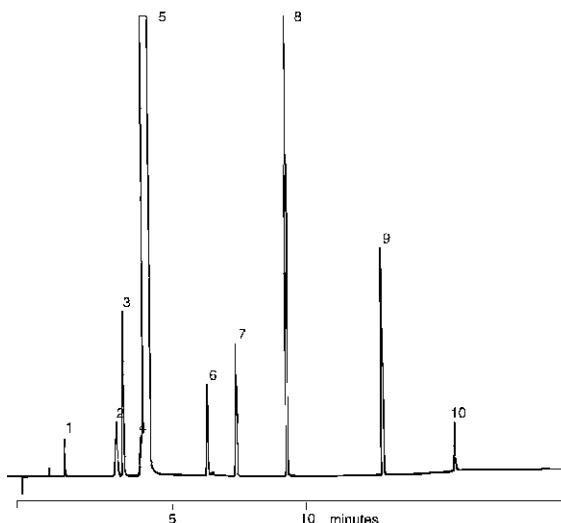




GC Columns and Applications

## FLA 14 | Analysis of Lavender Oil on BPX5



Column Part No.:	054101	Average Linear Velocity:	36 cm/sec at 40 °C
Phase:	BPX5, 0.25 µm film	Injection Mode:	Split
Column:	30 m x 0.25 mm ID	Split Ratio:	200:1
Initial Temp.:	40 °C, 1 min	Purge on (Split)	
Rate 1:	5 °C/min to 260 °C	Vent Flow:	200 mL/min
Final Temp.:	260 °C	Injection Volume:	0.2 µL
Detector Type:	Mass Spectrometer	Injection Temp.:	250 °C
Carrier Gas:	He, 7.0 psi	Liner Type:	4 mm ID Double Taper Liner
Carrier Gas Flow:	1.0 mL/min	Liner Part Number:	092018
Constant Flow:	On		

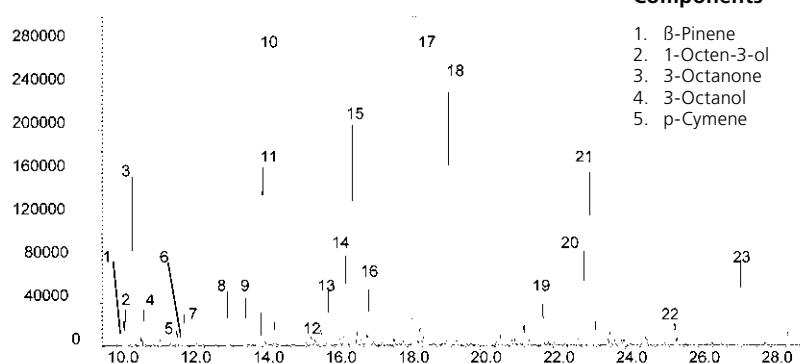**Components**

1. β-Pinene
2. 1-Octen-3-ol
3. 3-Octanone
4. 3-Octanol
5. p-Cymene
6. Limonene
7. cis-Ocimene
8. cis-Linalool oxide
9. Trans-Linalool oxide
10. Linalool L
11. Octenyl acetate
12. Camphor
13. Lavandulol
14. Borneol L
15. Terpinen-4-ol
16. α-Terpineol
17. Linalyl acetate
18. Lavundyl Acetate
19. Geranyl Acetate
20. α-Santalene
21. β-Caryophyllene
22. α-Cadinene
23. α-Caryophyllene oxide

## FLA 03 | Analysis of Orris Concentrate on BP20

Column Part No.:	054436
Column:	BP20, 0.5 µm
Phase:	25 m x 0.32 mm I.D.
Initial Temp.:	70 °C, 1 min
Rate:	10 °C/min
Final Temp.:	250 °C, 10 min
Carrier Gas:	Helium
Carrier Pressure:	10 psi
Injection Mode:	Split 50:1

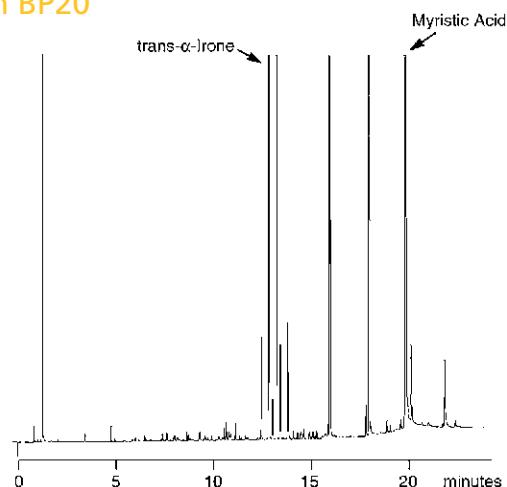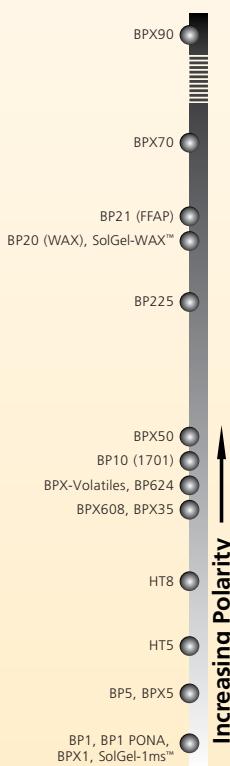


## FLA 21 | Analysis of Spearmint Oil on SolGel-WAX™



GC Columns and Applications

Column Part No.:	054796
Phase:	SolGel-WAX™, 0.25 µm film
Sample:	Neat
Column:	30 m x 0.25 mm ID
Initial Temp.:	40 °C, 1 min.
Rate 1:	8 °C/min to 220 °C
Final Temp.:	220 °C, 5 min.
Detector Type:	Mass Spectrometer
Carrier Gas:	He, 25.7 psi
Carrier Gas Flow:	1.8 mL/min.

Constant Flow:	On
Average Linear Velocity:	35 cm/sec at 40 °C
Injection Mode:	Split
Split Ratio:	100:1
Injection Volume:	0.2 µL
Injection Temp.:	250 °C
Liner Type:	4 mm ID Single Taper Liner
Liner Part Number:	092017
Full Scan / SIM:	Full scan 45-450

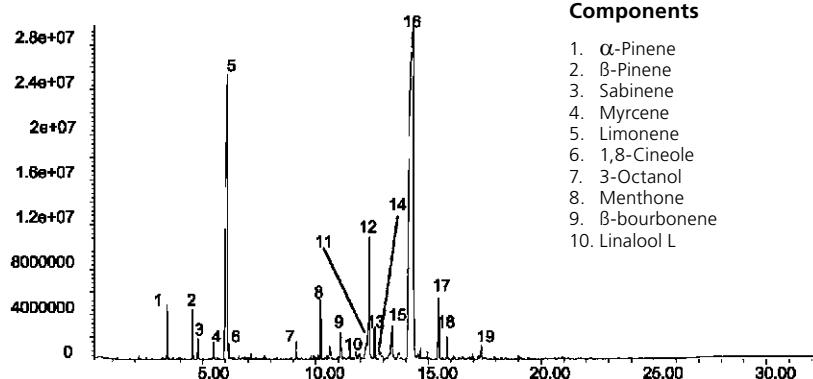


### Components

- 1.  $\alpha$ -Pinene
- 2.  $\beta$ -Pinene
- 3. Sabinene
- 4. Myrcene
- 5. Limonene
- 6. 1,8-Cineole
- 7. 3-Octanol
- 8. Menthone
- 9.  $\beta$ -bourbonene
- 10. Linalool L
- 11. trans Caryophyllene
- 12. cis dihydrocarvone
- 13. Trans dihydrocarvone
- 14. Menthol
- 15. Dihydrocarvyl acetate
- 16. L-Carvone
- 17. trans Carveol
- 18. cis Carveol
- 19. Caryophyllene oxide

## FLA 18 | Analysis of Ylang Ylang Oil on SolGel-WAX™

Column Part No.:	054796
Phase:	SolGel-WAX™, 0.25 µm
Sample:	Ylang Ylang oil neat.
Column:	30 m x 0.25 mm ID
Initial Temp.:	40 °C, 2 min.
Rate 1:	3 °C/min to 250 °C
Final Temp.:	250 °C, 10 min.
Detector Type:	Mass Spectrometer
Carrier Gas:	He, 25.7 psi
Carrier Gas Flow:	1.8 mL/min.

Constant Flow:	On
Average Linear Velocity:	35 cm/sec at 40 °C
Injection Mode:	Split
Split Ratio:	120:1
Injection Volume:	0.1 µL
Injection Temp.:	250 °C
Autosampler:	No
Liner Type:	4 mm ID Double Taper Liner
Liner Part Number:	092018
Full Scan / SIM:	Full scan 45-450

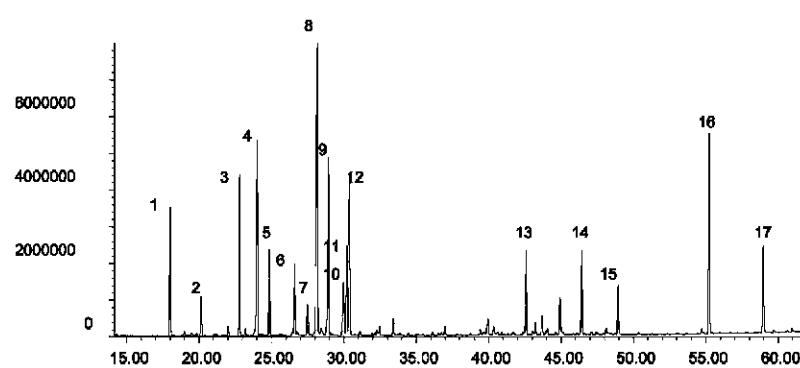

### Components

- 1. p-Methyl anisole
- 2.  $\alpha$ -Copaene
- 3. Linalool L
- 4.  $\beta$ -Caryophyllene
- 5. Methyl benzoate
- 6.  $\alpha$ -Humulene
- 7.  $\alpha$ -Amorphene
- 8. Germacrene
- 9. Benzyl acetate
- 10.  $\delta$ -Cadinene
- 11.  $\alpha$ -Farnesene
- 12. Geranyl acetate
- 13. trans-Cinamyl acetate
- 14. Farnesyl acetate
- 15. Farnesol
- 16. Benzyl benzoate
- 17. Benzyl salicylate




GC Columns and Applications

## FLA 16 | Analysis of Pine Oil on BPX5

Column Part No.:	054101
Phase:	BPX5, 0.25 µm film
Column:	30 m x 0.25 mm ID
Initial Temp.:	40 °C, 1 min.
Rate 1:	5 °C/min to 260 °C
Final Temp.:	260 °C
Detector Type:	Mass Spectrometer
Carrier Gas:	He, 7.0 psi
Carrier Gas Flow:	1.0 mL/min.
Constant Flow:	On

Average Linear Velocity:	36 cm/sec at 40 °C
Injection Mode:	Split
Split Ratio:	200:1
Purge on (Split)	
Vent Flow:	200 mL/min.
Injection Volume:	0.2 µL
Injection Temp.:	250 °C
Liner Type:	4 mm ID Double Taper Liner
Liner Part Number:	092018

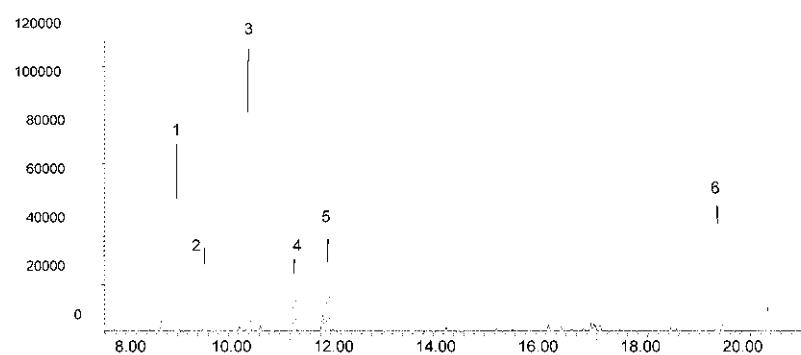



## Components

1. α-Pinene
2. Camphene
3. β-Pinene
4. δ-3-Carene
5. Limonene
6. Endobornyl acetate

## FLA 15 | Analysis of Tea Tree Oil on BPX5

Column Part No.:	054101
Phase:	BPX5, 0.25 µm film
Column:	30 m x 0.25 mm ID
Initial Temp.:	40 °C, 1 min.
Rate 1:	5 °C/min to 200 °C
Final Temp.:	200 °C
Detector Type:	Mass Spectrometer
Carrier Gas:	He, 7.0 psi
Carrier Gas Flow:	1.0 mL/min.
Constant Flow:	On

Average Linear Velocity:	36 cm/sec at 40 °C
Injection Mode:	Split
Split Ratio:	200:1
Purge on (Split)	
Vent Flow:	200 mL/min.
Injection Volume:	0.2 µL
Injection Temp.:	250 °C
Liner Type:	4 mm ID Double Taper Liner
Liner Part Number:	092018

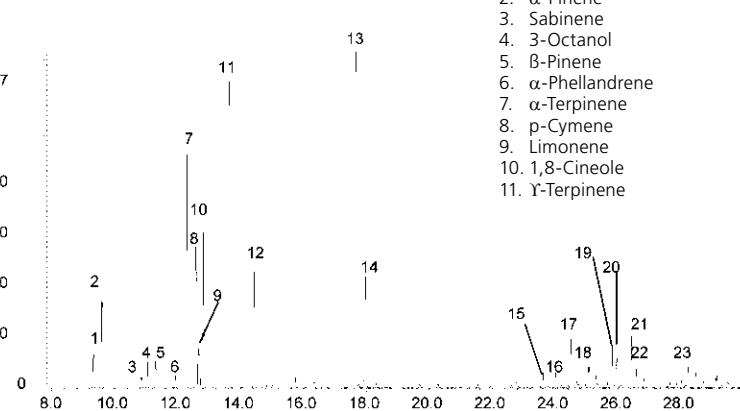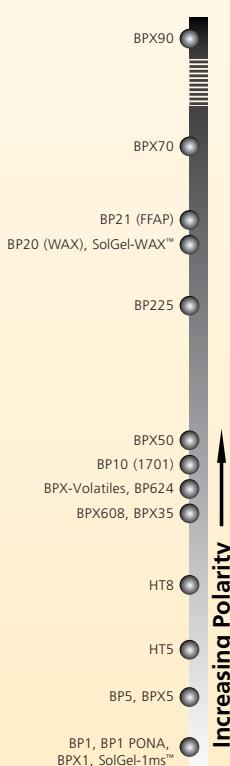

## Components


1. Thujene
2. α-Pinene
3. Sabinene
4. 3-Octanol
5. β-Pinene
6. α-Phellandrene
7. α-Terpinene
8. p-Cymene
9. Limonene
10. 1,8-Cineole
11. γ-Terpinene
12. Terpinolene
13. Terpinen-4-ol
14. α-Terpineol
15. α-Gurjunene
16. (trans)-β-Caryophyllene
17. Aromadendrene
18. Alloaromadendrene
19. Ledene
20. Germacrene B
21. δ-Cadinene
22. 1s, cis-Calamenene
23. Globulol

## FLA 12 | Analysis of Nutmeg Oil on BPX5

Column Part No.:	054101	Constant Flow:	On
Phase:	BPX5, 0.25 µm film	Average Linear Velocity:	36 cm/sec at 40 °C
Column:	30 m x 0.25 mm ID	Injection Mode:	Split
Initial Temp.:	40 °C, 1 min.	Split Ratio:	200:1
Rate:	5 °C/min to 260 °C,	Purge on (Split) Vent Flow:	200 mL/min.
Final Temp.:	260 °C	Injection Volume:	0.2 µL
Detector Type:	Mass Spectrometer	Injection Temp.:	250 °C
Carrier Gas:	He, 7.0 psi	Liner Type:	4 mm ID Double Taper Liner
Carrier Gas Flow:	1.0 mL/min.	Liner Part Number:	092018



GC Columns and Applications

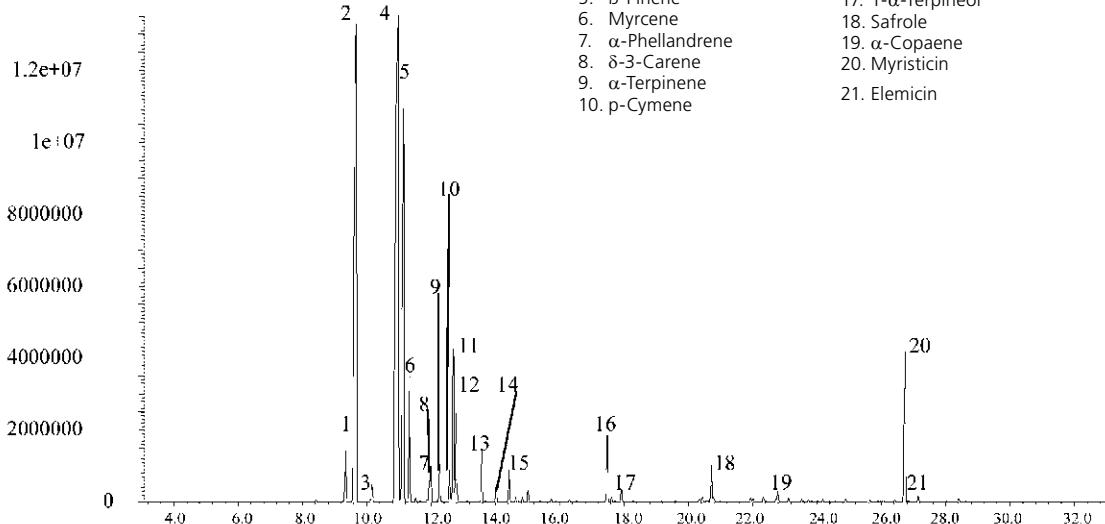

### Components

- |                           |                            |
|---------------------------|----------------------------|
| 1. $\alpha$ -Thujene      | 11. Limonene               |
| 2. $\alpha$ -Pinene       | 12. $\beta$ -Phellandrene  |
| 3. Camphene               | 13. $\gamma$ -Terpinene    |
| 4. Sabinene               | 14. trans-Sabinene hydrate |
| 5. $\beta$ -Pinene        | 15. $\alpha$ -Terpinolene  |
| 6. Myrcene                | 16. Terpinen-4-ol          |
| 7. $\alpha$ -Phellandrene | 17. 1- $\alpha$ -Terpineol |
| 8. $\delta$ -3-Carene     | 18. Safrole                |
| 9. $\alpha$ -Terpinene    | 19. $\alpha$ -Copaene      |
| 10. p-Cymene              | 20. Myristicin             |
|                           | 21. Elemicin               |






GC Columns and Applications

## FLA 13 | Analysis of Rosemary Oil on BPX5


**Column Part No.: 054101**

Phase:	BPX5, 0.25 µm film
Column:	30 m x 0.25 mm ID
Initial Temp.:	40 °C, 1 min.
Rate 1:	5 °C/min to 260 °C,
Final Temp.:	260 °C
Detector Type:	Mass Spectrometer
Carrier Gas:	He, 7.0 psi
Carrier Gas Flow:	1.0 mL/min.
Constant Flow:	On

Average Linear Velocity:	36 cm/sec at 40 °C
Injection Mode:	Split
Split Ratio:	200:1
Purge on (Split)	
Vent Flow:	200 mL/min.
Injection Volume:	0.2 µL
Injection Temp.:	250 °C
Liner Type:	4 mm ID Double Taper Liner
Liner Part Number:	092018

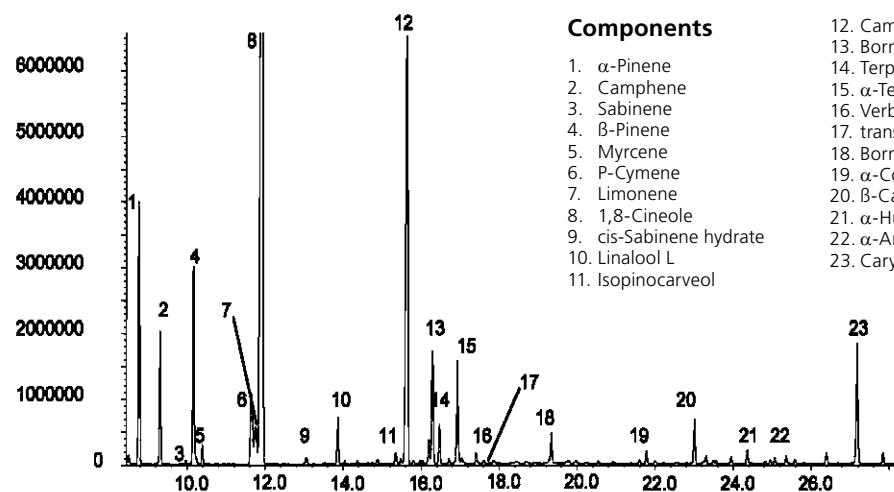**Components**

- |                         |                         |
|-------------------------|-------------------------|
| 1. α-Pinene             | 12. Camphor             |
| 2. Camphene             | 13. Borneol L           |
| 3. Sabinene             | 14. Terpinen-4-ol       |
| 4. β-Pinene             | 15. α-Terpineol         |
| 5. Myrcene              | 16. Verbenone           |
| 6. P-Cymene             | 17. trans-(+)-Carveol   |
| 7. Limonene             | 18. Bornyl acetate      |
| 8. 1,8-Cineole          | 19. α-Copaene           |
| 9. cis-Sabinene hydrate | 20. β-Caryophyllene     |
| 10. Linalool L          | 21. α-Humulene          |
| 11. Isopinocarveol      | 22. α-Amorphene         |
|                         | 23. Caryophyllene oxide |

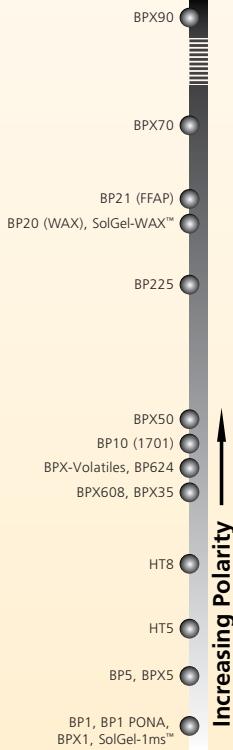

## FLA 22 | Analysis of Tasmanian Lavender Oil on SolGel-WAX™




GC Columns and Applications

### Column Part No.:

**054796**

Phase:	SolGel-WAX™, 0.25 µm film
Sample:	Neat
Column:	30 m x 0.25 mm ID
Initial Temp.:	40 °C, 1 min.
Rate 1:	8 °C/min to 220 °C,
Final Temp.:	220 °C, 5 min.
Detector Type:	Mass Spectrometer
Carrier Gas:	He, 25.7 psi
Carrier Gas Flow:	1.8 mL/min.

Constant Flow:	On
Average Linear Velocity:	35 cm/sec at 40 °C
Injection Mode:	Split
Split Ratio:	100:1
Injection Volume:	0.2 µL
Injection Temp.:	250 °C
Liner Type:	4 mm ID Single Taper Liner
Liner Part Number:	092017
Full Scan / SIM:	Full scan 45-450

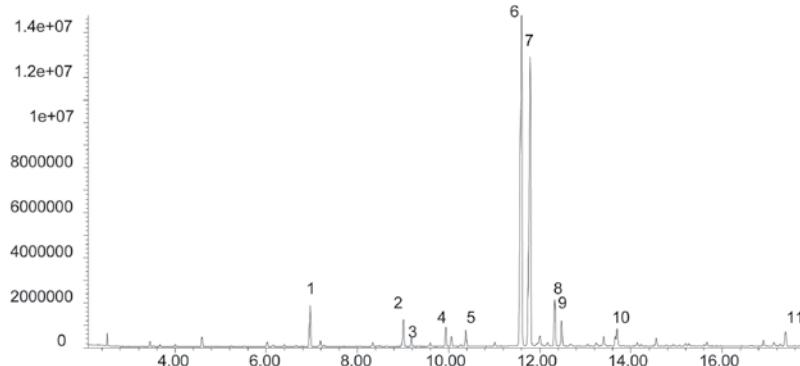

### Components

1. 3-Octanone
2. Octenyl acetate
3. Octanol
4. Cis Linalool oxide
5. Trans Linalool Oxide
6. Linalool L
7. Linalyl acetate
8. Terpinen-4-ol
9. Lavandulyl acetate
10. Borneol L
11. Caryophyllene oxide



GC Columns and Applications


## ENV 54 | Total Recoverable Petroleum Hydrocarbons (TRPH) Analysis on Standard and Fast BPX5

Column Part No.:	054101
Phase:	BPX5, 0.25 µm film
Column:	30 m x 0.25 mm ID
TRPH (C8-C40):	5 ng/ µL in dichloromethane
Initial Temp:	40 °C , 2 min
Rate 1:	30 °C/min to 330 °C
Rate 2:	N/A
Final Temp.:	330 °C, 9 min
Detector Type:	FID, 350 °C
Carrier Gas:	He, 14.1 psi
Carrier Gas Flow :	1.29 mL/min
Constant Flow:	On
Average Linear Velocity:	40 cm/sec at 40 °C
Injection Mode:	Split, 120:1
Purge On Time:	N/A
Purge On (Split) Vent Flow:	160 mL/min
Injection Volume:	1 µL
Injection Temperature:	250 °C
Autosampler:	Yes
Liner Type :	4 mm ID FocusLiner™ with single taper
Liner Part Number:	092003

Column Part Number:	054099
Phase:	BPX5, 0.10 µm film
Column:	10 m x 0.10 mm ID
TRPH (C8-C40) Standard:	5 ng/ µL in dichloromethane
Initial Temp.:	40 °C , 1 min
Rate 1:	30 °C/min to 330 °C
Rate 2:	N/A
Final Temp.:	330 °C, 0 min
Detector Type:	FID, 350 °C
Carrier Gas:	He, 28 psi
Carrier Gas Flow :	0.52 mL/min
Constant Flow:	On
Average Linear Velocity:	55 cm/sec at 40 °C
Injection Mode:	Split, 120:1
Purge On Time:	N/A
Purge On (Split) Vent Flow:	62 mL/min
Injection Volume:	1 µL
Injection Temperature:	250 °C
Autosampler:	Yes
Liner Type :	2.3 mm ID FocusLiner™
Liner Part Number:	092005


### NORMAL

Chromatogram showing separation of Total Recoverable Petroleum Hydrocarbons using a conventional 30 meter x 0.25 mm ID BPX5 column with a 0.25 micron film.

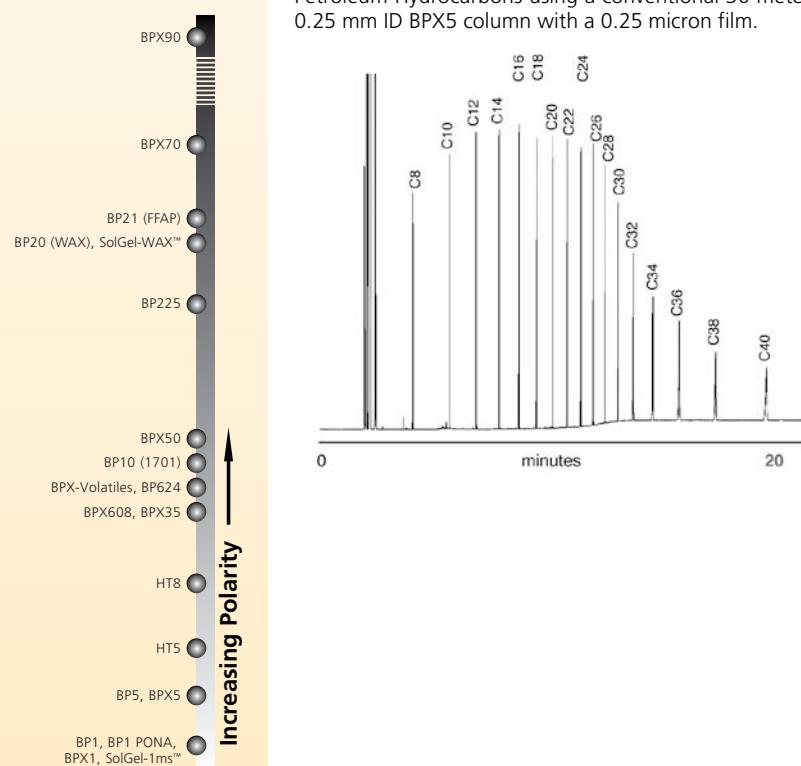

### FAST

Chromatogram showing separation of Total Recoverable Petroleum Hydrocarbon using a FAST BPX5 column.

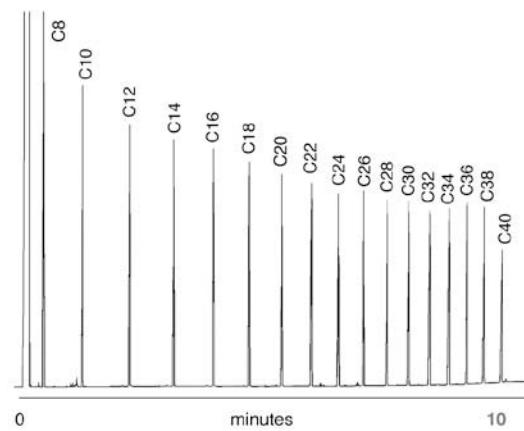


# PET 01 | Analysis of Gasoline Range Hydrocarbons on BP1-PONA



GC Columns and Applications

Column Part No.:	054950	Temp. 3:	120 °C
Phase:	BP1 PONA	Rate 3:	10 °C/min
Column:	50 m x 0.15 mm ID	Final Temp.:	190 °C
Initial Temp.:	30 °C, 5 min hold	Detector:	FID
Rate 1:	2 °C/min	Sensitivity:	32 x 10-12 AFS
Temp. 2:	80 °C	Injection Mode:	Split
Rate 2:	50 °C/min	Carrier Gas:	H <sub>2</sub> , 40 psi

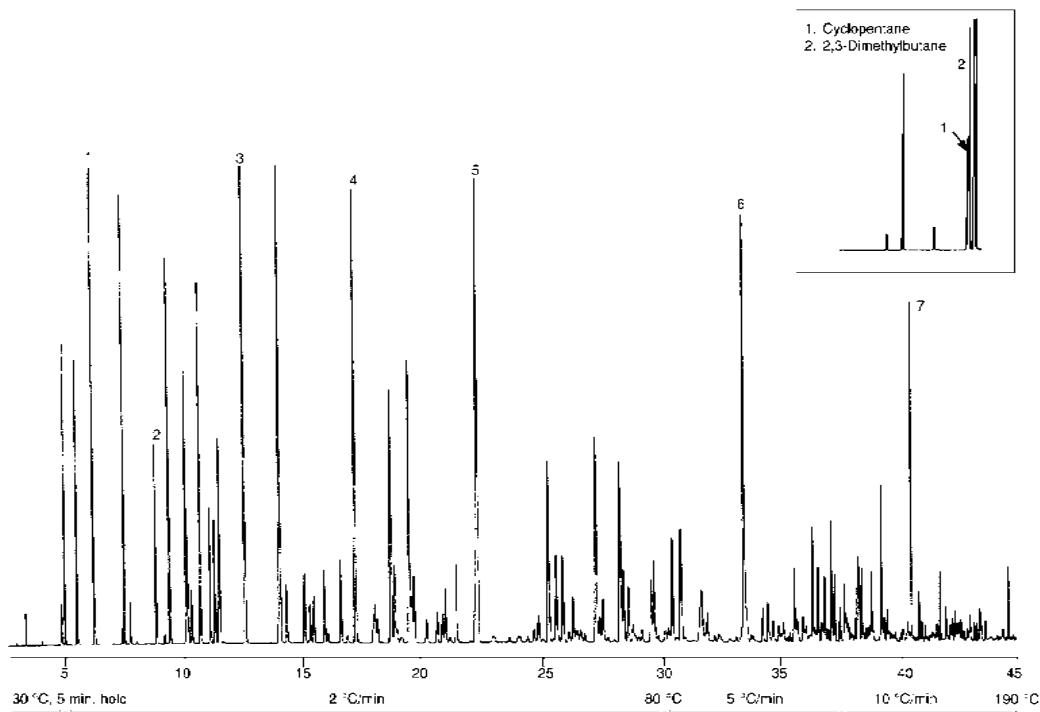

## Components


TIME COMPOUND	18.43 2-Methyl-3-ethylpentane	28.84 1-cis-2-trans-4-trans-Trimethylcyclohexane
4.85 Cyclopentane	18.84 2-Methylheptane	28.95 1-cis-2-trans-4-cis-Trimethylcyclohexane
5.00 2,3-Dimethylbutane	19.69 1-Methyl-2-ethylcyclopentane	29.16 3,4-Dimethylheptane
5.25 2-Methylpentane	18.98 4-Methylheptane	29.31 3-Methylethylhexane
5.74 3-Methylpentane	19.23 1-cis-2-cis-4-trans-Trimethylcyclopentane	29.68 4-Methyloctane
1. 6.45 n-Hexane	19.74 3-Methylheptane	29.81 2-Methyloctane
7.46 2,2-Dimethylpentane	19.77 1-trans-4-Dimethylcyclohexane	30.56 3-Methyloctane
7.60 Methylcyclopentane	20.73 1-Methyl-cis-2-ethylcyclopentane	30.93 o-Xylene
7.91 2,4-Dimethylpentane	20.86 1-Methyl-trans-3-ethylcyclopentane	31.75 1-Methyl-2-propylcyclopentane
8.18 2,2,3-Trimethylbutane	21.08 1-Methyl-cis-3-ethylcyclohexane	and 1-Methyl-trans-4-ethylcyclohexane
2. 8.99 Benzene	21.27 1-Ethy-1-methycyclopentane	31.98 1-Methyl-cis-4-ethylcyclohexane
9.35 3,3-Dimethylpentane	21.53 1-trans-2-Dimethylcyclohexane	32.46 3,3-Diethylpentane
9.55 Cyclohexane	5. 22.43 n-Octane	32.89 2,2,6-Trimethylheptane
10.23 2-Methylhexane	23.05 iso-Propylcyclopentane	33.17 1,1,2-Trimethylcyclohexane
10.32 2,3-Dimethylpentane	24.14 2,2,5-Trimethylhexane	6. 33.52 n-Nonane
10.47 1,1-Dimethylcyclohexane	24.19 2,2,4-Trimethylhexane	34.26 iso-Propylbenzene
10.83 3-Methylhexane	24.53 2,4,4-Trimethylhexane	34.48 tert-Butylcyclopentane
11.23 1-trans-3-Dimethylcyclopentane	24.79 2,3,5-Trimethylhexane	34.68 tert-Butylbenzene
11.43 1-cis-3-Dimethylcyclopentane	25.16 2,4-Dimethylheptane	35.57 sec-Butylcyclopentane
11.55 3-Ethylpentane	25.41 n-Propylcyclopentane	36.33 3-Methylnonane
11.63 1-trans-2-Dimethylcyclopentane	25.73 1-cis-2-Dimethylcyclohexane	36.56 n-Propylbenzene
11.78 2,2,4-Trimethylpentane	26.00 1,1,3-Trimethylcyclohexane	36.83 n-Propylcyclohexane
3. 12.73 n-Heptane	26.25 2,5-Dimethylheptane	37.12 m-Ethyltoluene
14.23 Methylcyclohexane	26.44 3,3-Dimethylheptane	37.24 p-Ethyltoluene
14.53 2,2-Dimethylhexane	26.58 3,5-Dimethylheptane	37.64 1,3,5-Trimethylbenzene
15.27 Ethylcyclopentane	26.77 4,4-Dimethylheptane	38.20 2-Methylnonane
15.49 2,5-Dimethylhexane	26.94 2,3,3-Trimethylhexane	38.36 o-Ethyltoluene
15.65 2,4-Dimethylhexane	27.43 Ethylbenzene	38.75 3,6-Dimethyloctane
16.09 1-trans-2-cis-4-Trimethylcyclopentane	27.57 1-cis-3-cis-5-Trimethylpentane	38.75 1,2,4-Trimethylbenzene
16.24 2,3,4-Trimethylpentane	27.69 1,1,4-Trimethylcyclohexane	7. 40.32 n-Decane
16.78 1-trans-2-cis-3-Trimethylcyclopentane	27.88 2,3,4-Trimethylhexane	40.63 1,2,3-Trimethylbenzene
17.05 2,3,3-Trimethylpentane	28.15 3,3,4-Trimethylhexane	41.57 4-Methyldecane
4. 17.39 Toluene	28.42 m-Xylene	41.94 sec-Butylbenzene
18.27 2,3-Dimethylhexane	28.54 p-Xylene	42.45 n-Butylbenzene




GC Columns and Applications

## PET 11 | Analysis of Crude Oil and Wax Mixtures on HT5

<b>Column Part No.:</b>	<b>054635</b>	Final Temp.:	480 °C
Phase:	HT5, 0.1 µm	Carrier Gas:	H <sub>2</sub> , 15 psi
Column:	12 m x 0.22 mm I.D. (Aluminum Clad)	Detector:	F.I.D.
Initial Temp.:	35 °C	Sensitivity:	32 x 10 -12 AFS
Program Rate:	10 °C/min.	Injection Mode:	Split

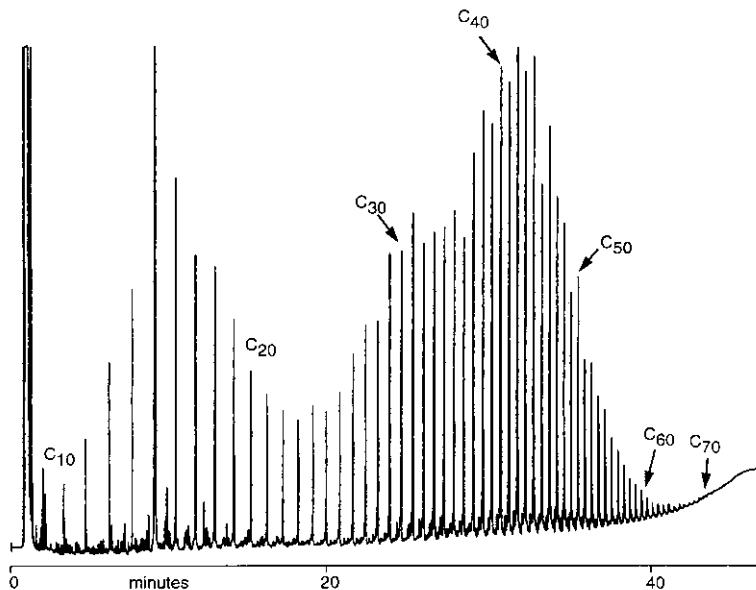Notes: HT5 is the best column for the analysis of hydrocarbons C<sub>10</sub> - C<sub>70</sub>.


## PET 26 | Standard for D2887 on BPX1

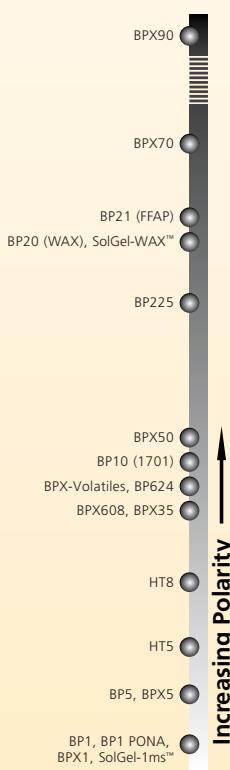

<b>Column Part No.:</b>	<b>054802</b>	Final Temp.:	350 °C, 10min
Phase:	BPX1, 2.65 µm film	Detector Temp.:	400 °C
Column:	10 m x 0.53 mm ID	Carrier Gas:	He, 20 mL/min
Initial Temp.:	40 °C	Instrument:	HP 6890
Rate:	15 °C/min		

**Separation Systems Injector**

Initial Temp.:	80 °C
Rate:	15 °C/min
Final Temp.:	350 °C, 10 min

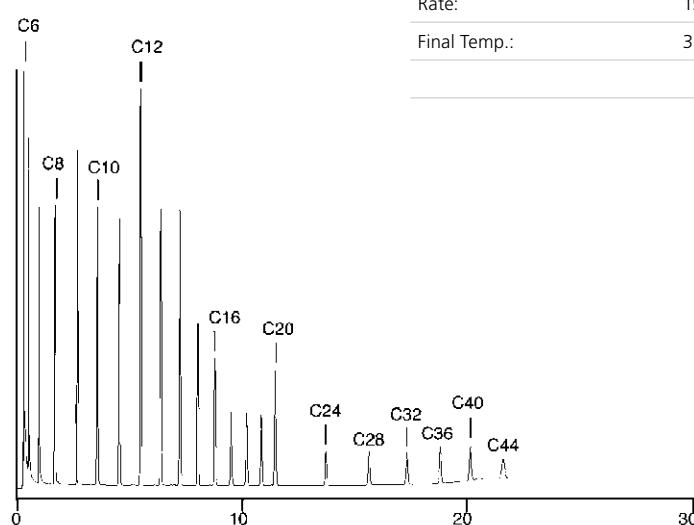

## ENV 51 | Total Recoverable Petroleum Hydrocarbons (TRPH) C8-C40 on SolGel-1ms™




GC Columns and Applications

### Column Part No.: 054795

Phase:	SolGel-1, 0.25 µm film 30 m x 0.25 mm ID	Pressure:	16.6 psi
Sample Introduction:	Split / Splitless	Column Flow:	1.6 mL/min
Injector Temp.:	250 °C	Linear Velocity:	35 cm/sec at 40 °C
Injection Volume:	0.5 µL	Initial Temp.:	40 °C
Autosampler Syringe:	5 µL Fixed Needle Part No. 001810	Initial Time:	2 min
Septa:	Auto-Sep T™ Part No. 041882	Rate 1:	30 °C/min
Injection Type:	Split	Final Temp. 1:	310 °C
Purge On Time:	NA	Hold Time:	0 min
Purge On (Spilt) Vent:	100 mL/min	Rate 2:	10 °C/min
Split Ratio:	62.5 to 1	Final Temp. 2:	340 °C
Liner Type:	Double taper Part No. 092018	Hold Time:	0 min
Carrier Gas:	He	Run Time:	22.00 min
Constant Flow:	On	Detector Type:	FID at 340 °C


Sample Description: TRPH mix 500 mg/L, 4 ng per component on column.

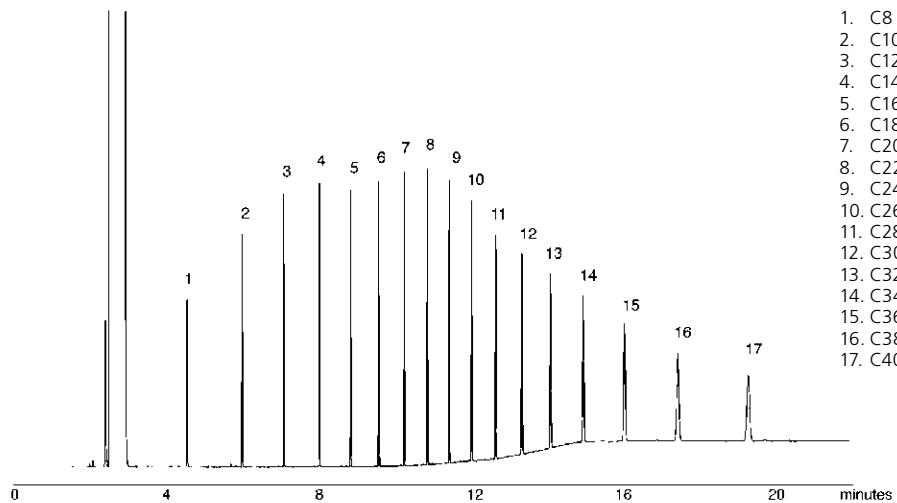

### Components

1. C8
2. C10
3. C12
4. C14
5. C16
6. C18
7. C20
8. C22
9. C24
10. C26
11. C28
12. C30
13. C32
14. C34
15. C36
16. C38
17. C40

## PET 27 | Analysis of Polywax 1000 on an Aluminum Clad HT5

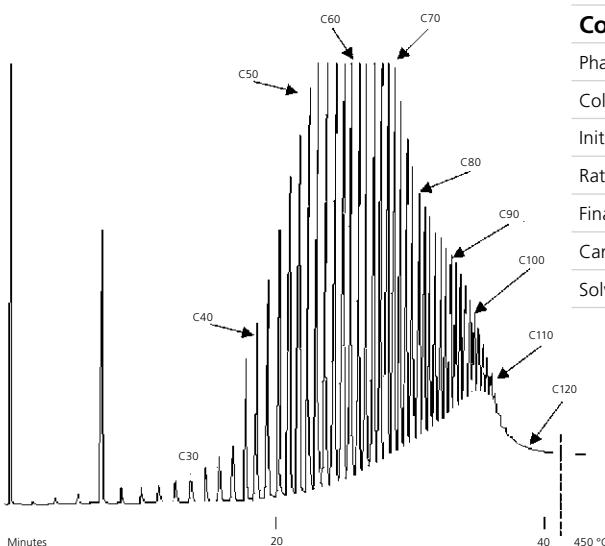


### Column Part No.: 054673

Phase:	HT5, 0.075 µm film
Column:	5 m x 0.53 mm ID
Initial Temp.:	40 °C, 1 min
Rate:	10 °C/min
Final Temp.:	450 °C, 10 min
Carrier Gas:	He, 20 mL/min
Solvent:	CS <sub>2</sub>





GC Columns and Applications

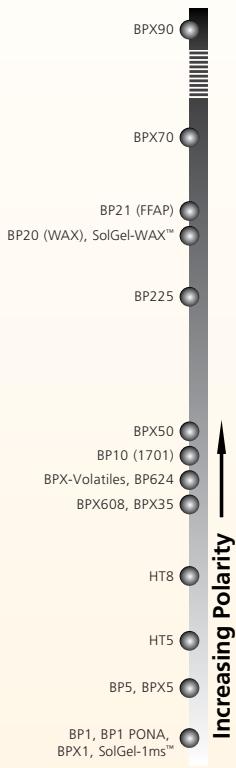

## PET 22 | Unleaded Gasoline on BPX5


Column Part No.:	<b>054101</b>
Phase:	BPX5, 0.25 µm film
Column:	30 m x 0.25 mm ID
Sample Introduction:	Split / Splitless
Injector Temp.:	240 °C
Injection Volume:	0.1 µL
Autosampler Syringe:	0.5 µL Removable Needle Part No. 000410
Septa:	Auto-Sep T™ Part No. 041882
Injection Type:	Split
Purge On Time:	NA
Purge On (Split) Vent:	200 mL/min
Split Ratio:	149 to 1
Liner Type:	FocusLiner™ single taper Part No. 092003
Carrier Gas:	He

Constant Flow:	On
Pressure:	13.6 psi
Column Flow:	1.34 mL/min
Linear Velocity:	30 cm/sec at 25 °C
Initial Temp.:	25 °C
Initial Time:	1 min
Rate 1:	30 °C/min
Final Temp. 1:	240 °C
Hold Time:	1 min
Run Time:	9.17 min
Final Temp. 2:	340 °C
Hold Time:	0 min
Run Time:	22.00 min
Detector Type:	FID at 280 °C

Sample Description: Pure Unleaded Gasoline

**Components**


1. Benzene
2. Toluene
3. Ethylbenzene
4. m, p - Xylene
5. o - Xylene

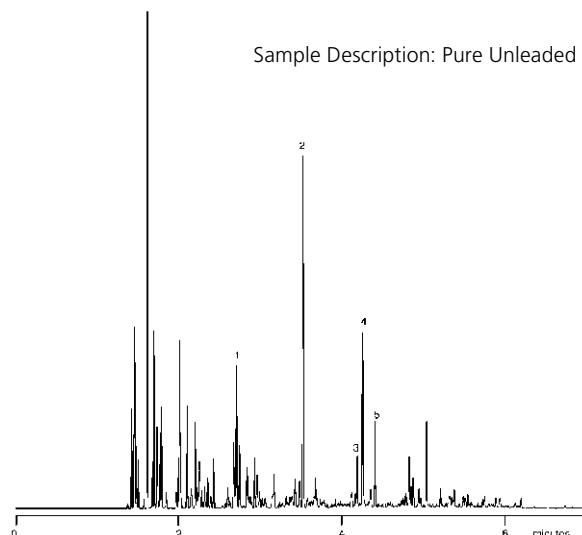

## PET 18 | Analysis of Polywax 655 on Megabore BPX1

Column Part No.:	<b>054800</b>
Phase:	BPX1, 0.1 µm
Column:	5 m x 0.53 mm ID
Initial Temp.:	40 °C
Rate:	15 °C

Final Temp.:	420 °C, 5 min
Detector Temp.:	440 °C
Carrier:	He, 10 mL/min
Instrument:	HP 6890
Solvent:	CS <sub>2</sub>

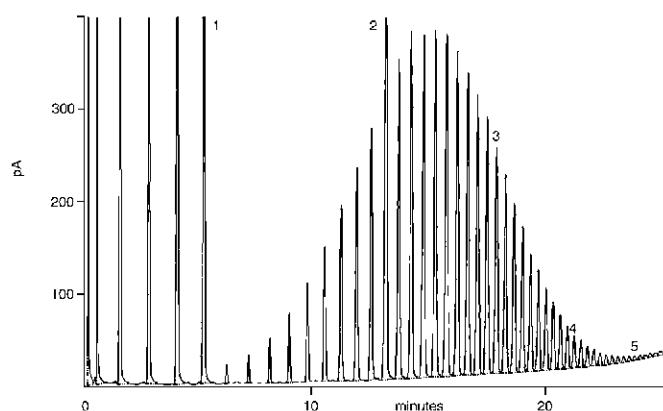


## PET 06 | Analysis of Polywax 655 and Refinery Lubrication Oil on HT5



GC Columns and Applications

Column Part No.:	<b>054661</b>
Phase:	HT5, 0.1 µm
Column:	6 m x 0.53 mm ID
Initial Temp.:	50 °C
Rate:	10 °C/min
Final Temp.:	480 °C, 15 min
Detector:	FID
Sensitivity:	40 x 10 -12 AFS
Injection Mode:	On-Column
Carrier Gas:	Hydrogen, 20 ml/min
Solvent:	CS <sub>2</sub>

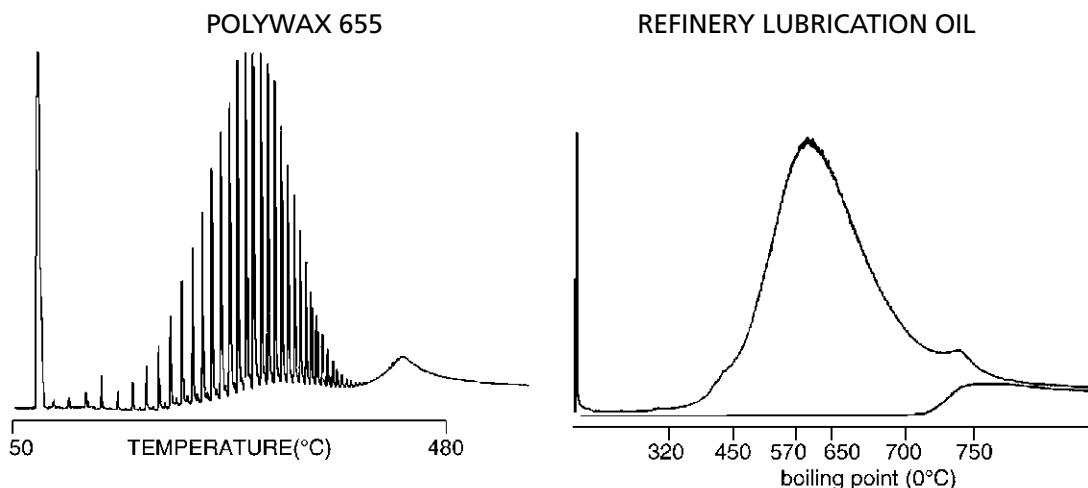

## ENV 54 | BPX1 A New Era in Simulated Distillation Technology (SimD)

Column Part No.:	<b>054800</b>
Phase:	BPX1, 0.1 µm
Column:	5 m x 0.53 mm ID
Initial Temp.:	40 °C
Rate:	15 °C
Final Temp.:	420 °C, 5 min.
Detector Temp.:	440 °C
Carrier Gas:	Helium, 10 mL/min
Instrument:	HP6890
Initial Temp.:	40 °C
Rate:	15 °C
Final Temp.:	420 °C, 5 min.

Data supplied by Dr. J. Lubkowitz and the staff at Separation Systems Inc.

Figure. 1. Standard mix for HTSD using BPX1-SimD


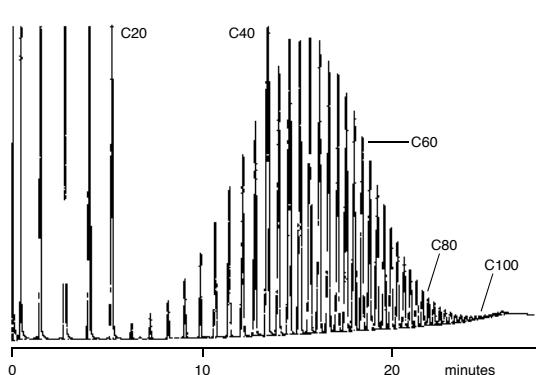


Figure. 2. Enlarged section of Figure 1.



# GC Application by Industry | General Chemistry


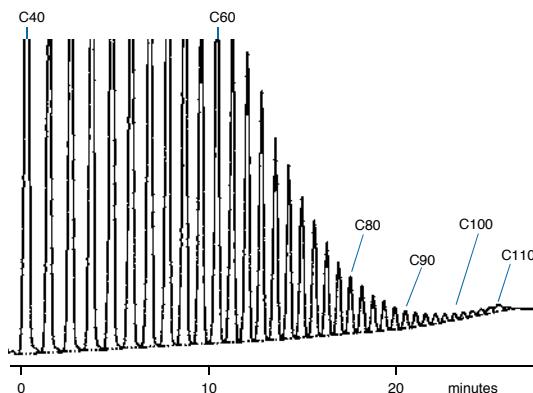


GC Columns and Applications

## ALC 02 | Analysis of 18 Alcohols on BP20

Column Part No.:	054427
Phase:	BP20, 0.25 µm film
Column:	30 m x 0.25 mm ID
Initial Temp:	45 °C, 2 min
Rate:	3 °C/min

Final Temp:	80 °C, 0 min
Detector:	FID
Sensitivity:	128 x 10 <sup>-12</sup> AFS
Injection Mode:	Split

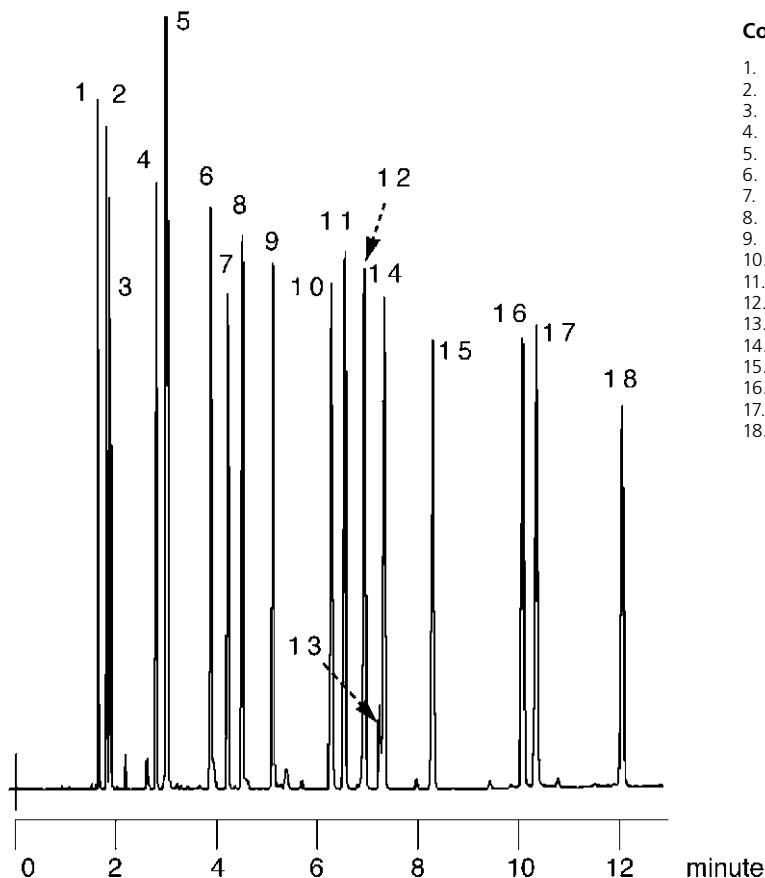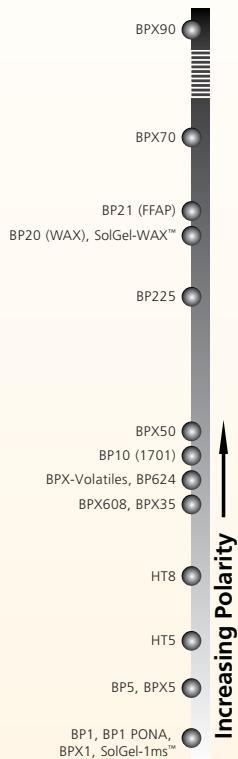


## ACI 03 | Analysis of 11 Organic Acids on BP20



GC Columns and Applications

Column Part No.:	054427
Phase:	BP20, 0.25 µm film
Column:	30 m x 0.25 mm ID
Initial Temp:	Isothermal at 155 °C

Detector:	FID
Sensitivity:	32 x 10 <sup>-12</sup> AFS
Injection Mode:	Split

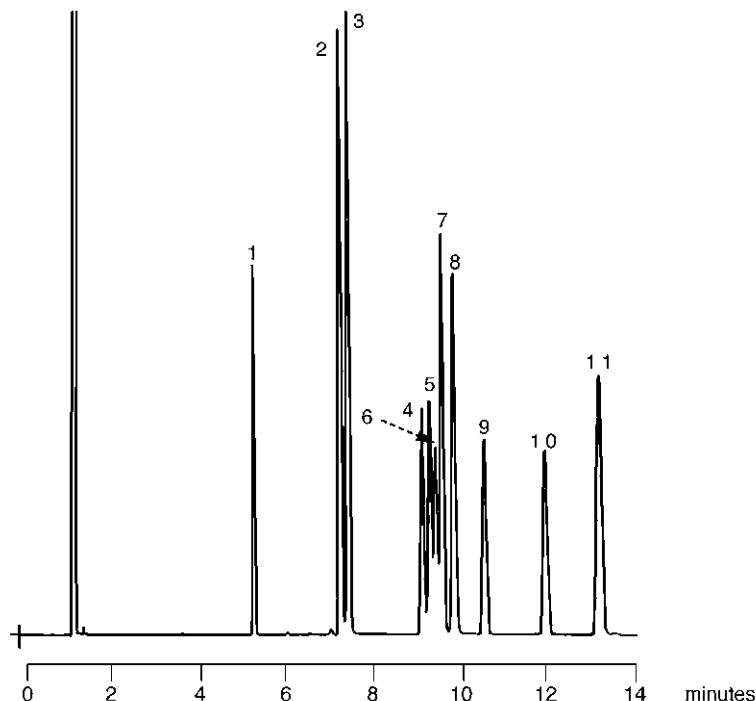

### Components

1. 2,6-Xylenol
2. o-Cresol
3. Phenol
4. o-Ethylphenol
5. 2,5-Xylenol
6. p-Cresol
7. 2,4-Xylenol
8. m-Cresol
9. 2-iso Propylphenol
10. 2,3-Xylenol
11. 3,5-Xylenol + p-Ethylphenol


Notes: BP20 column completely resolves the three cresol isomers.

## ACI 02 | Analysis of Organic Acids in Water on BP21

### Column Part No.: 054477

Phase:	BP21, 0.5 µm film	Final Temp:	180 °C, 5 min
Column:	30 m x 0.53 mm ID	Detector:	FID
Initial Temp:	85 °C, 0 min	Sensitivity :	64 x 10 <sup>-12</sup> AFS
Rate:	6 °C/min	Injection Mode:	On-Column

Notes: On-column injection and the addition of a 0.03 M Oxalic acid (2%) to the injection solution increases the acidity of the column to allow lactic acid to be detected.

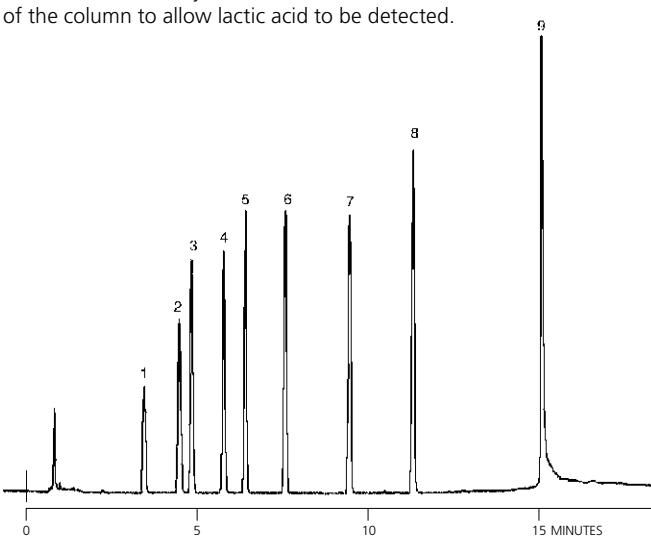


### Components

1. Acetic Acid
2. Propanoic Acid
3. iso-Butyric Acid
4. n-Butyric Acid
5. iso-Valeric Acid
6. n-Valeric Acid
7. n-Caproic Acid
8. n-Heptanoic Acid
9. Lactic Acid



## GC Columns and Applications

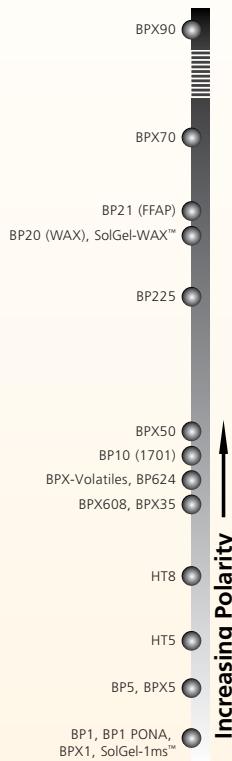


## AMI 06 | Analysis of Aromatic Amines from Diazo Dyes on BPX35

Column Part No:	054701
Phase:	BPX35 0.25 µm film
Azo Dyes standard:	10 ppm solution in DCM
Column:	30 m x 0.25 mm ID
Initial Temp:	50 °C, 2 min
Rate 1:	15 °C to 240 °C
Rate 2:	10 °C to 280 °C
Final Temp:	280 °C, 25 min
Detector Type:	MS D
Carrier Gas:	He, 7.1 psi
Carrier Gas Flow:	1.0 mL/min

Constant Flow:	On
Average Linear Velocity:	36 cm/sec at 50 °C
Injection Mode:	Splitless
Purge on Time:	1.0 min
Purge on (Split)	
Vent Flow:	60 mL/min
Injection Volume:	1 µL
Injection Temp:	250 °C
Liner Type:	4 mm ID Double Taper Liner
Liner Part No:	092018

## Components


1. Indolin
2. o-Toluidine
3. 2,4-Diaminoanisole
4. p-Chloroaniline
5. p-Cresidine
6. 2,4,6-Trimethylaniline
7. 4-Chlorotoluidine
8. Unknown
9. 2-Naphthylamine
10. Unknown
11. 4-Aminodiphenyl
12. 4,4'-Oxydianiline
13. 4,4'-Diaminodiphenylmethane
14. Benzidine
15. 3,3'-Dimethyl-4,4'-diaminodiphenylmethane
16. 3,3'-Dimethylbenzidine
17. 4,4'-Thiodianiline
18. 3,3'-Dichlorobenzidine
19. 4,4'-Methylene-bis (2-chloroaniline)
20. 3,3'-Dimethoxybenzidine

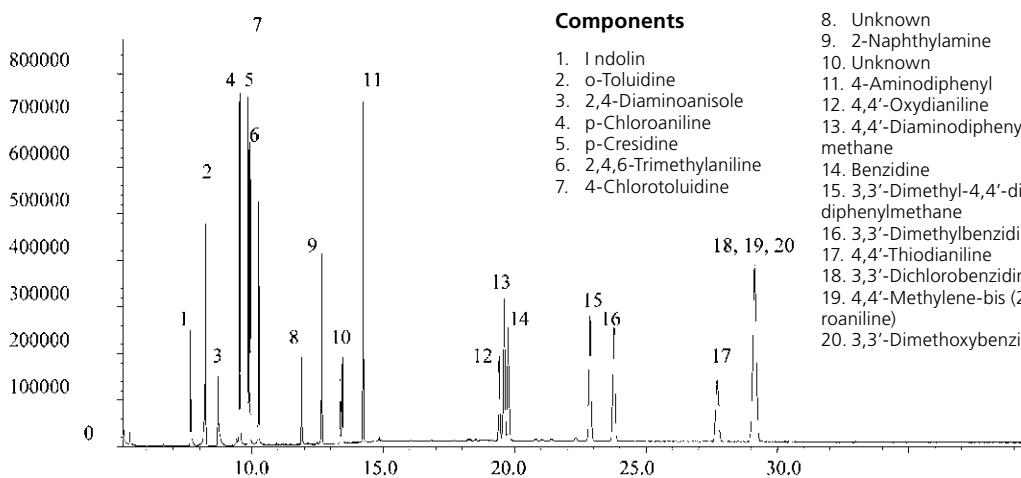

## AMI 03 | Analysis of Aromatic Amines on BP5

Column Part No.:	054197
Phase:	BP5, 1.0 µm film
Column:	12 m x 0.53 mm ID
Initial Temp:	60 °C, 0 min
Rate:	10 °C/min


Final Temp:	190 °C, 0 min
Detector:	FID
Sensitivity :	128 x 10-12 AFS
Injection Mode:	Split

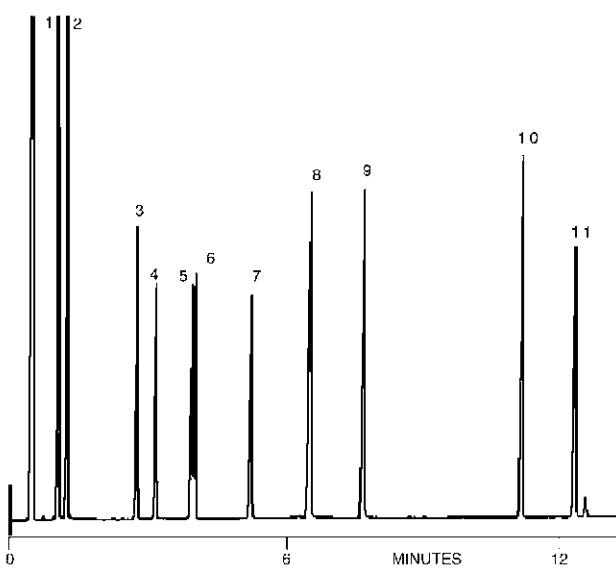

## Components

1. Pyridine
2. 2-Methyl Pyridine
3. Aniline
4. Benzylamine
5. o-Toluidine
6. m-Toluidine
7. 2,6-Dimethylaniline
8. 1,4-Phenyldiamine
9. Nicotine
10. Biphenylamine
11. Bibenzyllamine

## AMI 04 | Analysis of Amines on BP1

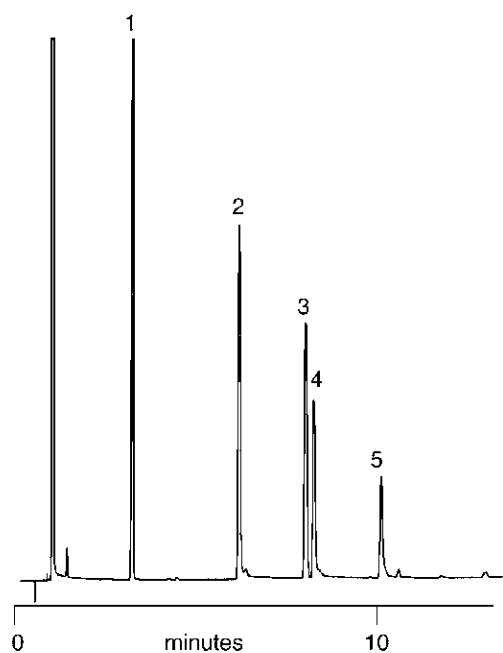

### Column Part No.: 054097

Phase:	BP1, 3.0 $\mu\text{m}$ film
Column:	12 m x 0.53 mm ID
Initial Temp:	70 °C
Rate:	10 °C/min
Final Temp.:	250 °C
Carrier Gas:	Nitrogen
Injection Volume:	0.1 $\mu\text{L}$

### Components

1. Aniline
2. Decylamine
3. Dicyclohexylamine
4. Dodecylamine
5. Tetradecylamine


## SOL 25 | Analysis of 22 Ketones on BPX35

### Column Part No.: 054701

Phase:	BPX35, 0.25 $\mu\text{m}$ film	Constant Flow:	On
Sample:	300 ppm in dichloromethane	Average Linear Velocity:	35 cm/sec at 40 °C
Column:	30 m x 0.25 mm ID	Injection Mode:	Split
Initial Temp:	40 °C, 5 min.	Split Ratio:	80:1
Rate:	10 °C/min to 170 °C	Injection Volume:	0.5 $\mu\text{L}$
Final Temp:	170 °C, 5 min.	Injection Temp.:	250 °C
Detector Type:	Mass Spectrometer	Liner Type:	4 mm ID Single Taper Liner
Carrier Gas:	He, 25.6 psi	Liner Part Number:	092017
Carrier Gas Flow:	1.6 mL/min.	Full Scan / SIM:	Full scan 45-450

### Components


- |                         |                         |                   |
|-------------------------|-------------------------|-------------------|
| 1. Acetone              | 7. 3-Methyl-2-pentanone | 15. 3-Heptanone   |
| 2. 2-Butanone           | 8. 3-Hexanone           | 16. 2-Heptanone   |
| 3. 3-Methyl-2-butane    | 9. 2-Hexanone           | 17. Cyclohexanone |
| 4. 2-Pentanone          | 10. Mesityl oxide       | 18. 2-Octanone    |
| 5. 3-Pentanone          | 11. 2-Methyl-3-hexanone | 19. 2-Nonanone    |
| 6. 4-Methyl-2-pentanone | 12. Cyclopentanone      | 20. 2-Decanone    |
|                         | 13. 4-Methyl-2-hexanone | 21. 2-Undecanone  |
|                         | 14. 5-Methyl-2-hexanone | 22. 2-Dodecanone  |

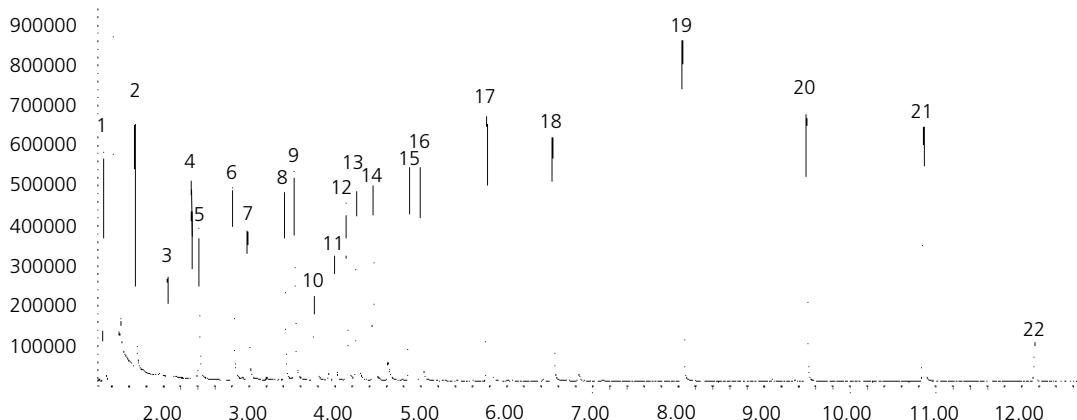

GC Columns and Applications



GC Columns and Applications

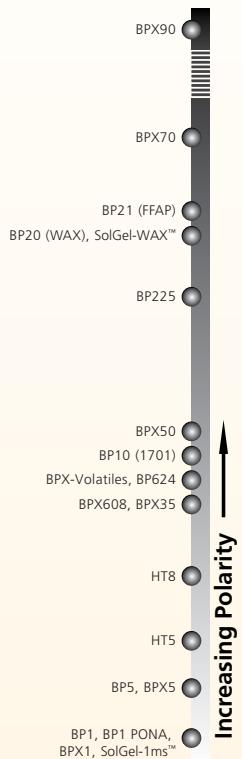


## SOL 33 | Analysis of Ketones on Thick Film BPX5

Column Part No.:	054123
Phase:	BPX5, 1.0 $\mu\text{m}$ film
Sample:	300 ppm in dichloromethane
Column:	60 m x 0.25 mm ID
Initial Temp.:	40 °C, 5 min.
Rate 1: 1	0 °C/min to 80 °C
Rate 2:	30 °C/min to 260 °C
Final Temp.:	260 °C, 4 min.
Detector Type:	FID
Detector Temp.:	360 °C

Carrier Gas:	He, 27.6 psi
Carrier Gas Flow:	1.9 mL/min.
Constant Flow:	On
Average Linear Velocity:	35 cm/sec at 40 °C
Injection Mode:	Split
Split Ratio:	100:1
Injection Volume:	0.4 $\mu\text{L}$
Injection Temp.:	250 °C
Liner Type:	4 mm ID Single Taper Liner
Liner Part Number:	092017

**Components**

- |                          |                         |                   |
|--------------------------|-------------------------|-------------------|
| 1. Ethanol               | 8. 3-Methyl-2-pentanone | 17. 2-Heptanone   |
| 2. Acetone               | 9. 3-Hexanone           | 18. Cyclohexanone |
| 3. 2-Butanone            | 10. 2-Hexanone          | 19. 2-Octanone    |
| 4. 3-Methyl-2-butanolone | 11. Mesityl oxide       | 20. 2-Nonanone    |
| 5. 2-Pantanone           | 12. Cyclopentanone      | 21. 2-Decanone    |
| 6. 3-pantanone           | 13. 2-Methyl-3-hexanone | 22. 2-Undecanone  |
| 7. 4-Methyl-2-pantanone  | 14. 4-Methyl-2-hexanone | 23. 2-Dodecanone  |
|                          | 15. 5-Methyl-2-hexanone |                   |
|                          | 16. 3-Heptanone         |                   |

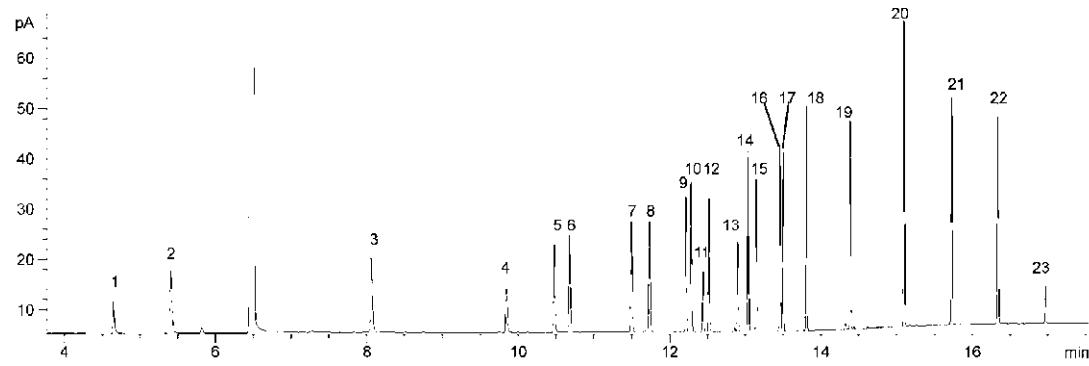


## ALC 09 | Analysis of Phenols Mixture on BPX35



GC Columns and Applications

### Column Part No: 054701

Phase:	BPX35, 0.25 µm film	Constant Flow:	On
Sample:	200 ppm in methanol	Average Linear Velocity:	35 cm/sec at 80 °C
Column:	30 m x 0.25 mm ID	Injection Mode:	Split
Initial Temp:	80 °C, 1 min	Split Ratio:	100:1
Rate 1:	10 °C/min to 300 °C	Injection Volume:	1 µL
Final Temp:	300 °C, 5 min	Injection Temperature:	250 °C
Detector Type:	Mass Spectrometer	Liner Type:	4 mm ID Single Taper Liner
Carrier Gas:	He, 29.2 psi	Liner Part No.:	092017
Carrier Gas Flow:	1.7 mL/min.	Full Scan / SIM:	Full scan 45-450

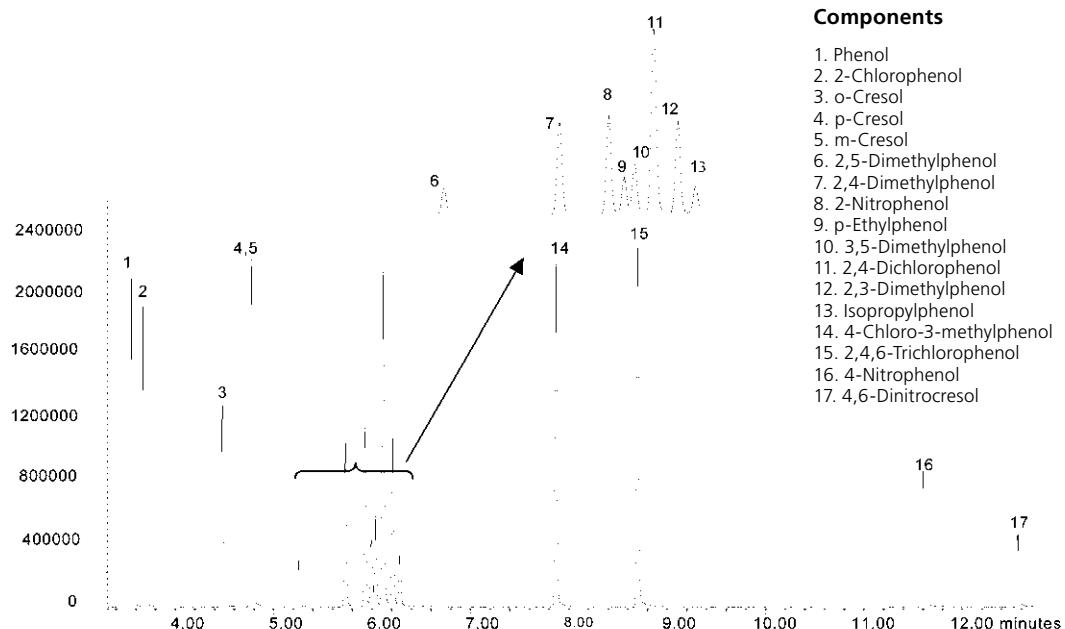

### Components

1. Phenol
2. 2-Chlorophenol
3. o-Cresol
4. p-Cresol
5. m-Cresol
6. 2,5-Dimethylphenol
7. 2,4-Dimethylphenol
8. 2-Nitrophenol
9. p-Ethylphenol
10. 3,5-Dimethylphenol
11. 2,4-Dichlorophenol
12. 2,3-Dimethylphenol
13. Isopropylphenol
14. 4-Chloro-3-methylphenol
15. 2,4,6-Trichlorophenol
16. 4-Nitrophenol
17. 4,6-Dinitrocresol



GC Columns and Applications




## POL 06 | Analysis of Various Monomers on SolGel-WAX™

Column Part No.:	054796
Phase:	SolGel-WAX, 0.25 µm film
Sample:	250 ppm in Hexane
Column:	30 m x 0.25 mm ID
Initial Temp:	40 °C, 1 min.
Rate 1:	10 °C/min to 250 °C
Final Temp:	250 °C,
Detector Type:	FID
Detector Temp.:	320 °C
Carrier Gas:	He, 16.6 psi

Carrier Gas Flow:	1.6 mL/min.
Constant Flow:	On
Average Linear Velocity:	35 cm/sec at 40 °C
Injection Mode:	Split
Split Ratio:	80:1
Injection Volume:	1 µL
Injection Temperature:	250 °C
Autosampler:	No
Liner Type:	4 mm ID Single Taper Liner
Liner Part Number:	092017

**Components**

1. Ethyl acrylate
2. n-Butyl acrylate
3. n-Butyl methacrylate
4. Styrene
5. 2-Ethylhexyl acrylate
6. Acrylic acid
7. Hydroxypropyl acrylate
8. Methacrylic acid
9. Unknown
10. Hydroxyethyl acrylate
11. Lauryl Methacrylate

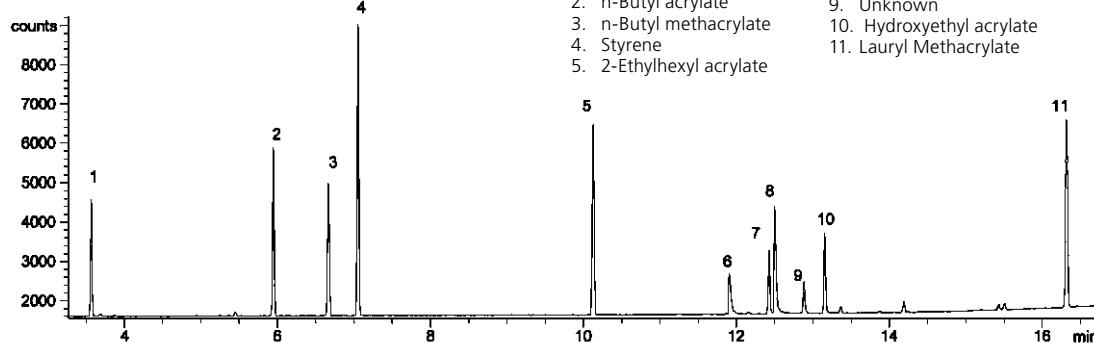


## POL 01 | Analysis of Unreacted Monomers in Latex on BP20

Column Part No.:	054488
Phase:	BP20, 1.0 µm
Column:	25 m x 0.53 mm ID
Initial Temp.:	40 °C, 2 min
Rate:	10 °C/min

Final Temp.:	230 °C, 5 min
Injector Cond.:	Split, 280 °C
Detector:	FID, 280 °C
Carrier Gas:	Hydrogen, 4 psi

Note: This was performed by heated headspace analysis.

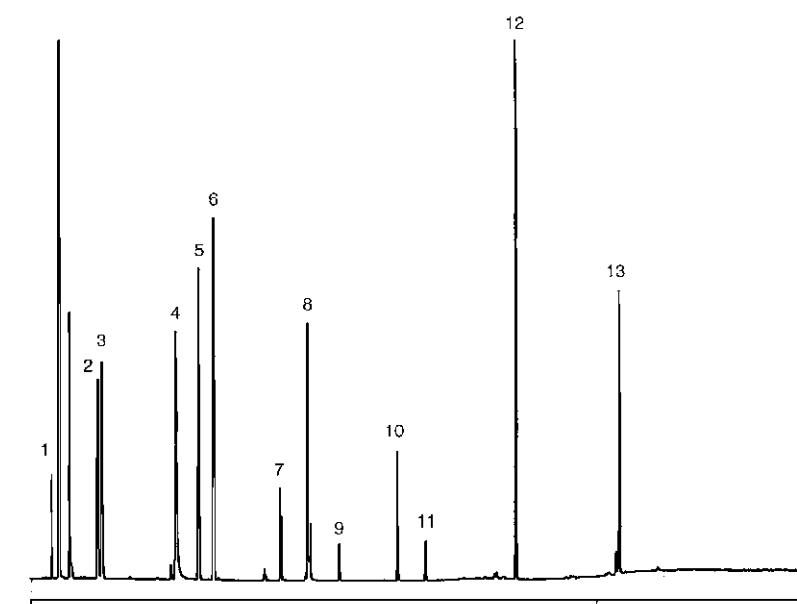**Components**

1. Vinyl Acetate
2. Ethyl Acrylate
3. Monomethyl Methacrylate
4. Butyl Acrylate
5. Butyl Methacrylate
6. Styrene
7. Di-methylamino Ethyl-methacrylate
8. 2-Ethyl Hexylacrylate
9. Octanol
10. Unknown
11. 2-(acetoacetoxy) Ethyl Methacrylate
12. Dibutyl Maleate
13. Dicyclopentenylmethoxyethyl Methacrylate



## POL 05 | Pyrolysis of Styrene-isoprene Copolymer Pyrolysis of Polystyrene on BP1



GC Columns and Applications

Column Part No.:	<b>054053</b>
Phase:	BP1, 1.0 $\mu\text{m}$
Column:	25 m x 0.22 mm ID
Initial Temp.:	40 °C, 1 min
Rate:	10 °C/min
Final Temp.:	140 °C
Detector:	FID
Pyrolysis Temp.:	550 °C
Carrier Gas:	H <sub>2</sub> , 10 psi


Column Part No.:	<b>054065</b>
Phase:	BP1, 0.5 $\mu\text{m}$
Column:	25 m x 0.32 mm ID
Initial Temp.:	40 °C, 1 min
Rate:	10 °C/min
Final Temp.:	130 °C
Detector:	FID
Pyrolysis Temp.:	800 °C
Carrier Gas:	H <sub>2</sub> , 5 psi

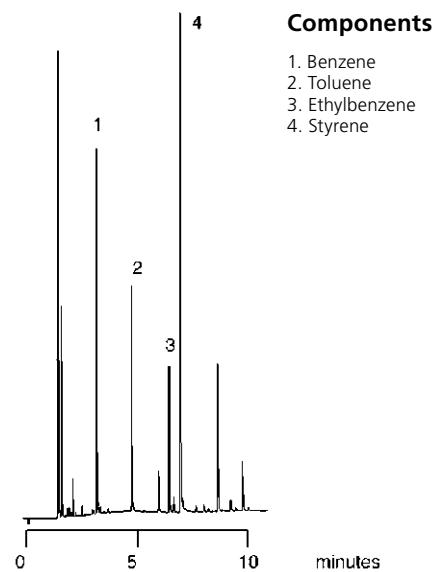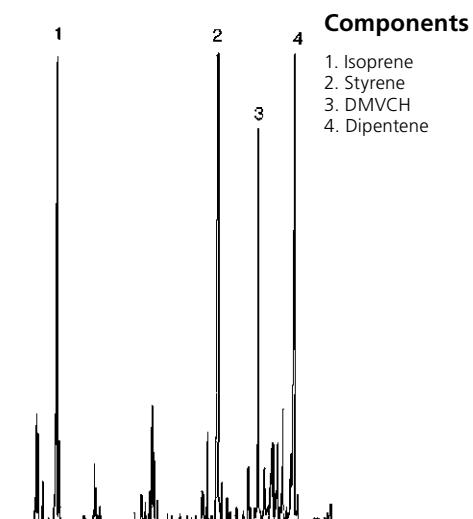

## SOL 21 | Analysis of a Common Solvent Mixture on BP624


Column Part No.:	<b>054832</b>
Phase:	BP624, 1.8 $\mu\text{m}$ film
Alcohol mix:	1000 ppm in Dimethyl Sulfoxide
Column:	30 m x 0.32 mm ID
Initial Temp.:	32 °C, 9 min.
Rate:	30 °C/min to 190 °C
Final Temp.:	190 °C, 0 min.
Detector Type:	FID
Carrier Gas:	He, 9.6 psi
Carrier Gas Flow:	2.2 mL/min.

Constant Flow:	On
Average Linear Velocity:	34 cm/sec at 32 °C
Injection Mode:	Split
Split Ratio:	100:1
Injection Volume:	0.2 $\mu\text{L}$
Injection Temperature:	250 °C
Autosampler:	No
Liner Type:	4 mm ID Double Taper Liner
Liner Part Number:	092018

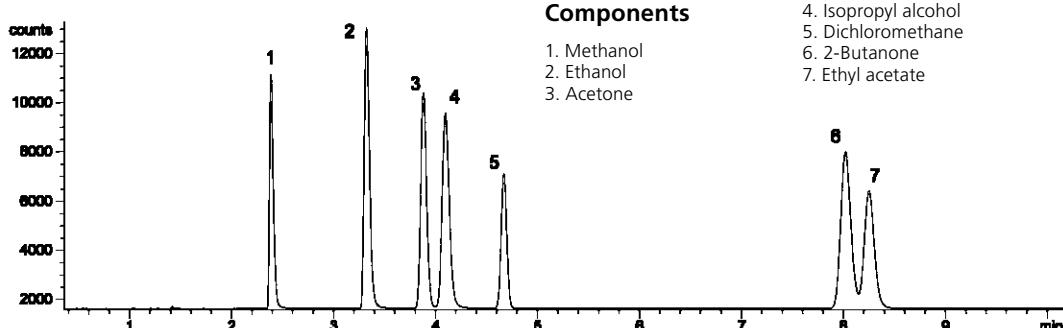




## GC Columns and Applications

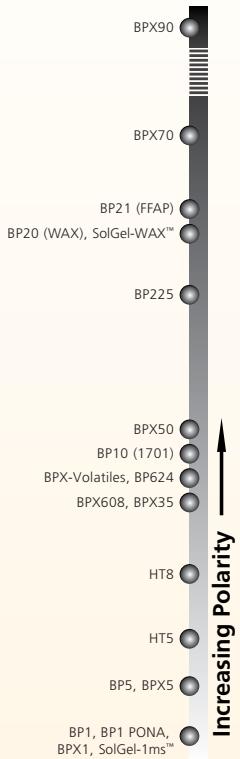

## ENV 52 | Industrial Solvents on SolGel-WAX™

Column Part No.	054797
Phase:	SolGel-WAX™, 0.5 µm film 30 m x 0.32 mm ID
Split / Splitless	
Injector Temp:	240 °C
Injection Volume:	0.1 µL
Autosampler Syringe:	0.5 µL Removable Needle Part No. 000410
Septa:	Auto-Sep T™ Part No. 041882
Injection Type:	Split
Purge On Time:	NA
Purge On (Split) Vent:	150 mL/min
Split Ratio:	83 to 1
Liner Type:	Single taper Part No. 092017
Carrier Gas:	He
Constant Flow:	On
Pressure:	8.4 psi
Column Flow:	1.84 mL/min
Linear Velocity:	30 cm/sec at 35 °C
Initial Temp.:	35 °C
Initial Time:	3 min
Rate 1:	15 °C/min
Final Temp .1:	230 °C
Hold Time:	4 min
Run Time:	20.00 min
Detector Parameters	
Detector Type:	FID at 270 °C

Sample Description: Industrial solvents mix, 25 to 50 ng per component on column

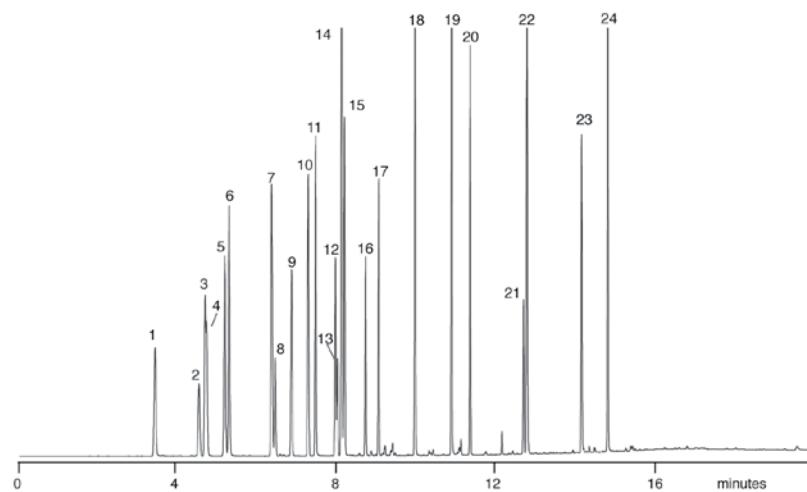

## Components

1. Acetone
2. Ethyl acetate
3. Methyl ethyl ketone
4. Contaminant
5. iso-Propanol
6. Ethanol
7. Methyl isobutyl ketone
8. Toluene
9. Butyl acetate
10. iso-butanol
11. Propylene glycol monomethyl ether
12. n-Butanol
13. Ethyl benzene
14. p-Xylene
15. m-Xylene
16. o-Xylene
17. Butyl Cellosolve acetate
18. Cyclohexanone
19. Butyl Cellosolve
20. Butyl glycol acetate
21. Hexyl Cellosolve
22. Isophorone
23. Butyl Carbitol
24. Benzyl alcohol


## SOL 04 | Acrylic Acid/Acrylamide Analysis on BP21

Column Part No.:	054473
Phase:	BP21, 0.5 µm film
Column:	12 m x 0.53 mm ID
Initial Temp:	75 °C, 0.5 min
Rate:	10 °C/min
Final Temp:	150 °C
Detector:	FID, 280 °C
Injection Mode:	On-Column
Carrier Gas:	He, 6 psi

Notes: When response of acrylic acid is low, removal of 30 cm from the front of the column will correct this loss. On-column injection is recommended or polymerization of acrylic acid may occur.

## Components




1. Acrylic acid (25 ng)
2. Acrylamide (10 ng)

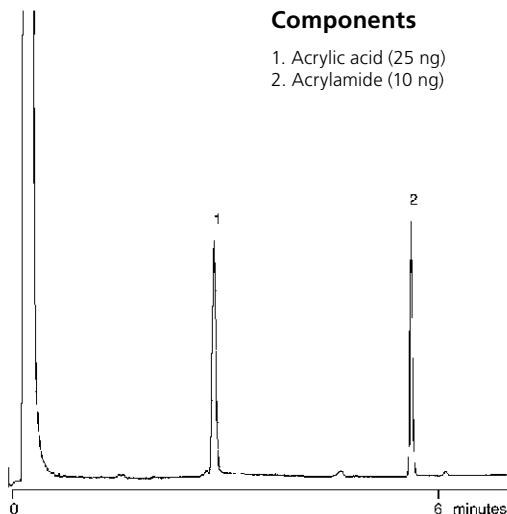

## TP-0138-C | Analysis Of Polybrominated Diphenyl Ethers on BP1






GC Columns and Applications

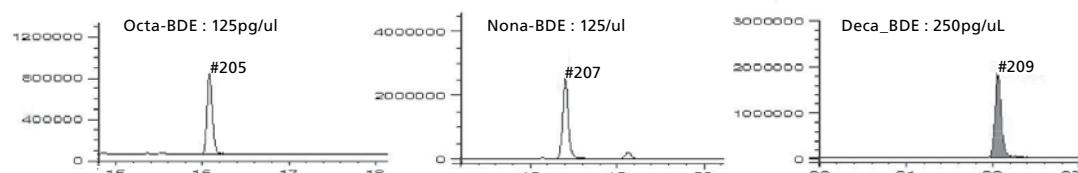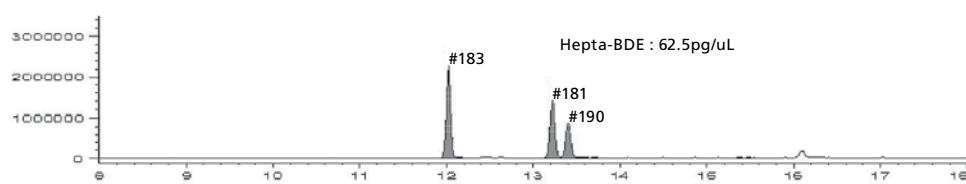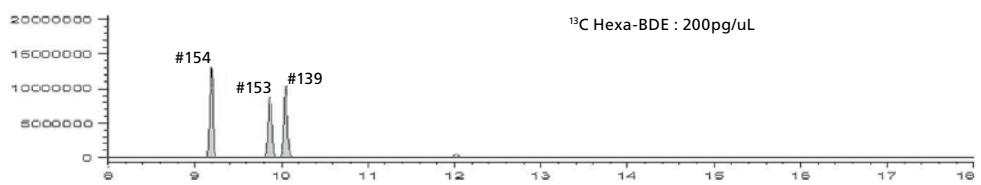

SGE would like to thank the Japan Food Research Centre for evaluating the BP1 column, SGE Japan and Chemicals Evaluation and Research Institute, Japan Toshiyuki KATAOKA, Masahiro AKIBA and Shinnichi KUDO.

## TP-0138-C | Analysis Of Polybrominated Diphenyl Ethers on BPX5

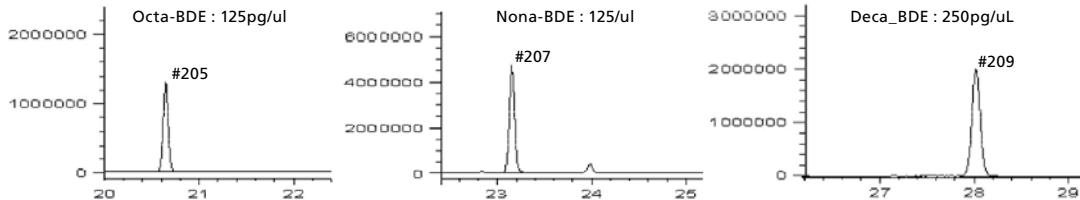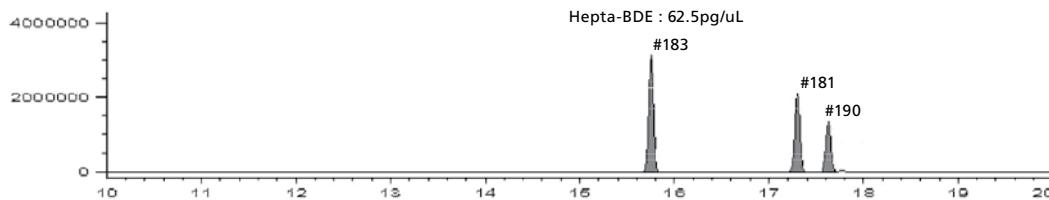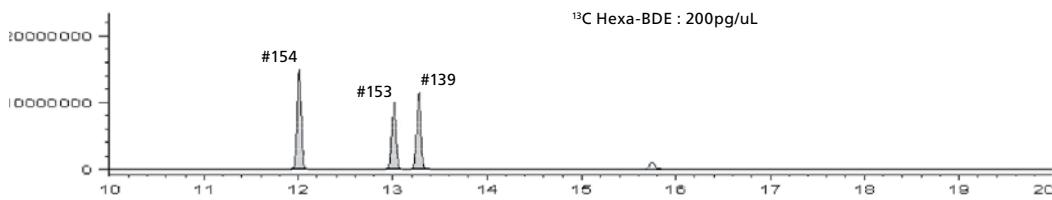


SGE would like to thank SGE Japan and Chemicals Evaluation and Research Institute, Japan Toshiyuki KATAOKA, Masahiro AKIBA and Shinnichi KUDO.



GC Columns and Applications

## TP-0138-C | Analysis Of A Mixture Of Pentachlorobiphenyls on HT8-PCB

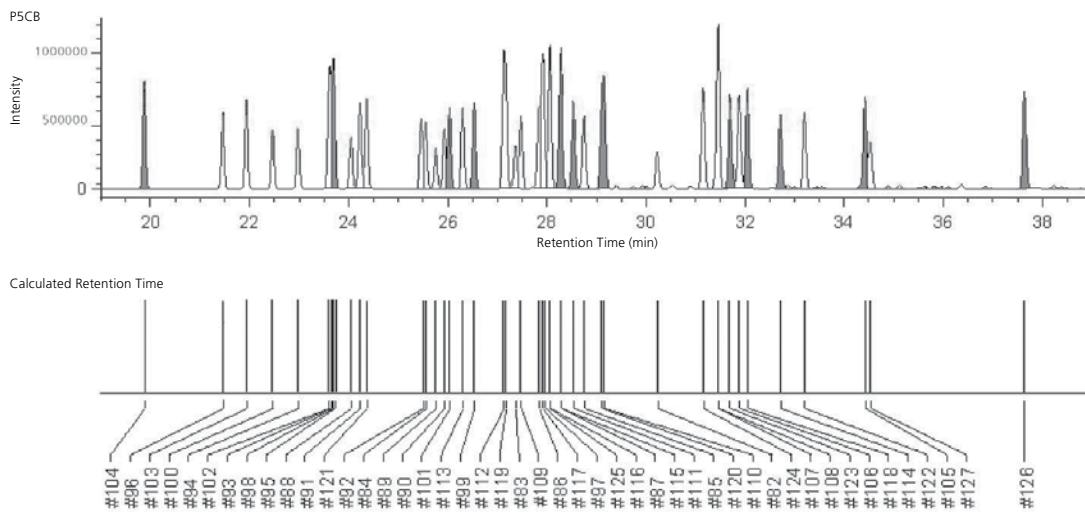

The separation of a mixture of pentachlorobiphenyls using an HT8-PCB column. Elution order calculated for the 5CBs from structure activity relationships based on coplanarity and confirmation, steric factors and electron density show a high correlation with experimental results.

SGE would like to thank T. Nakano, C. Matsumura and M. Tsurukawa at Hyogo Prefectural Institute of Public Health and Environmental Sciences, for providing the PCBs on HT8-PCB data.

## TP-0138-C | Analysis Of A Mixture Of PBDD, PCDD And PBDF on BPX70

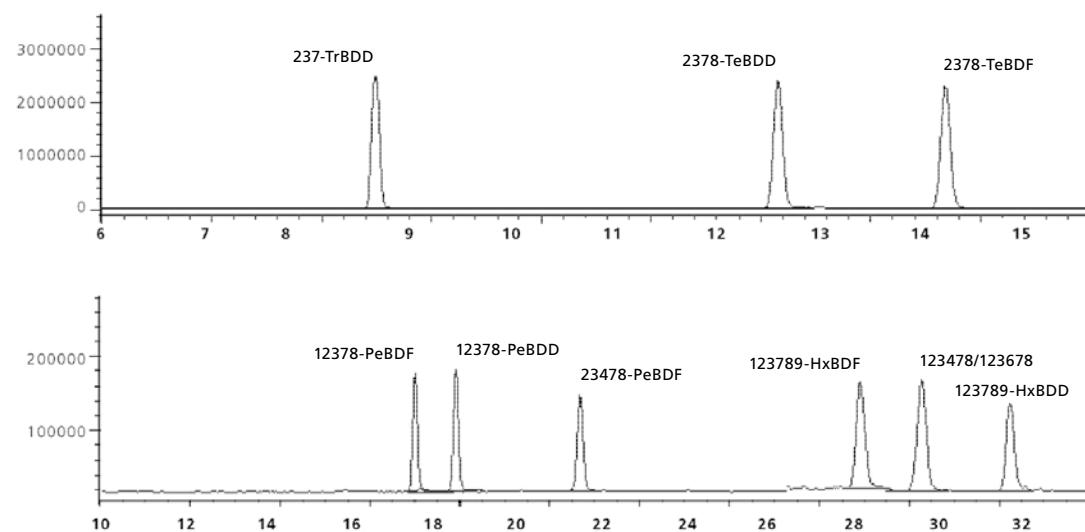


Figure 4. The separation of a mixture of PBDD and PBDF on a BPX70 column. The mixture was separated using the  $\pi-\pi$  interaction between the compounds and the cyano phase of the BPX70 column.

SGE would like to thank Toshiyuki Kataoka, Masahiro Akiba and Shinnichi Kudo of the Chemicals Evaluation and Research Institute, Japan, and SGE Japan, for providing the chromatograms of PBDEs on the ENV-5 and BPX70 columns.


# GC Application by Industry | Forensic

## PHA 14 | Analysis of Drugs of Abuse on BPX35

<b>Column Part No.:</b>	<b>054711</b>	<b>Temp 2:</b>	200 °C
Phase:	BPX35, 0.25 µm film	Rate 2:	7 °C/min
Column:	25 m x 0.22 mm ID	Temp 3:	295 °C
Initial Temp.:	80 °C	Rate 3:	20 °C/min
Rate 1:	15 °C/min	Final Temp.:	340 °C, 6 min



GC Columns and Applications

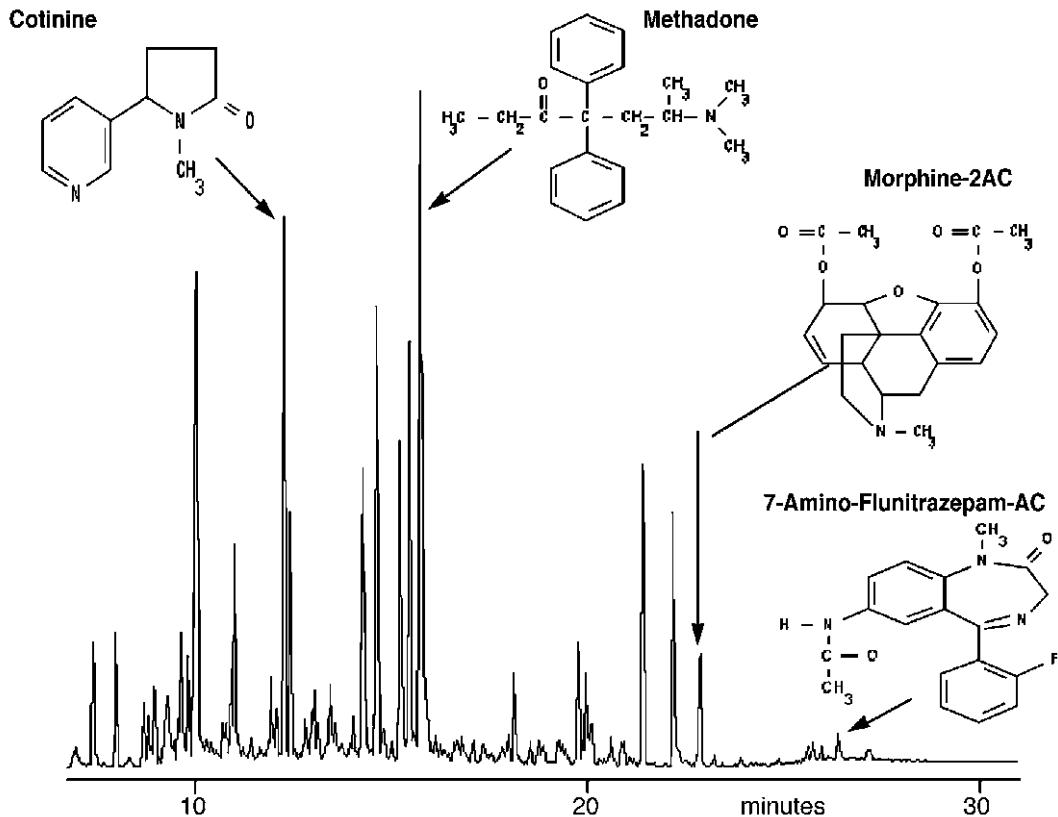


## PHA 09 | Analysis of Tricyclic Antidepressants on BPX35

<b>Column Part No.:</b>	<b>054711</b>
Phase:	BPX35, 0.25 µm
Column:	25 m x 0.22 mm ID
Initial Temp.:	210 °C, 1 min
Rate:	5 °C/min
Final Temp.:	280 °C
Carrier Gas:	Helium, 150 kpa
Injection Mode:	Split (20:1)
Detector:	FID, 380 °C

### Components


1. Amitriptyline
2. Trimipramine
3. Nortriptyline
4. Doxepin
5. Desipramine

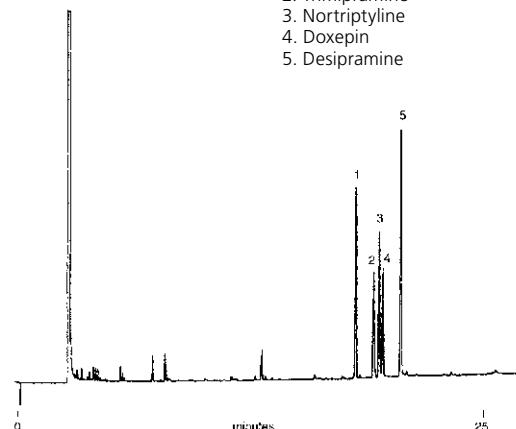

Note: BPX35 is a low bleed, chemically inert phase which allows trace analysis to occur.



## GC Columns and Applications

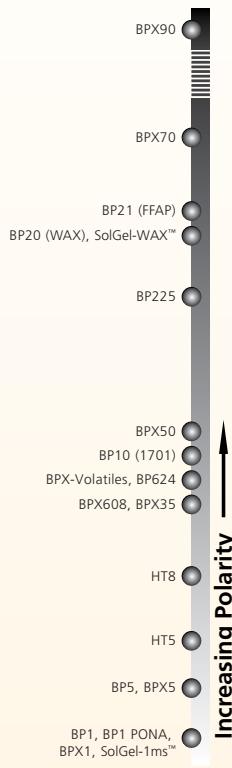


## PHA 19 | Analysis of a Variety of Antidepressant and Anticonvulsant Drugs on BPX50

**Column Part No.: 054751**

Phase: BPX50, 0.25 µm film  
 Column: 30 m x 0.25 mm ID  
 Sample: 5-10 ppm in methanol  
 Initial Temp: 150 °C, 0.5 min  
 Rate 1: 10 °C/min to 180 °C  
 Rate 2: 1.5 °C/min to 220 °C  
 Rate 2: 30 °C/min to 260 °C  
 Final Temp: 260 °C, 5 min  
 Detector Type: FID  
 Detector Temp.: 320 °C  
 Carrier Gas: He, 25.7 psi

Carrier Gas Flow: 1.8 mL/min.  
 Constant Flow: On  
 Average Linear Velocity: 35 cm/sec at 40 °C  
 Injection Mode: Splitless  
 Purge on Time: 0.5 min  
 Purge on (Split) Vent Flow: 60 mL/min  
 Injection Volume: 1 µL  
 Injection Temperature: 250 °C  
 Liner Type: 4 mm ID Single Taper Liner  
 Liner Part Number: 092017  
 Full Scan / SIM: Full scan 45-450

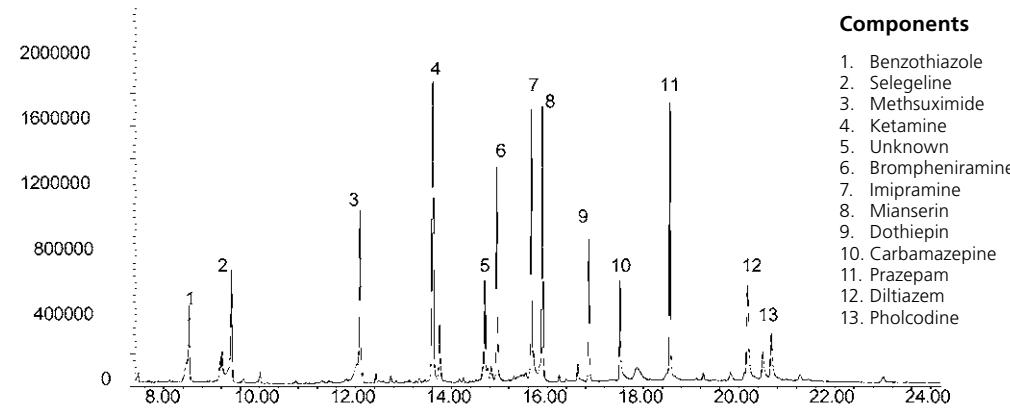**Components**

1. Benzothiazole
2. Selegeline
3. Methylsuximide
4. Ketamine
5. Unknown
6. Brompheniramine
7. Imipramine
8. Mianserin
9. Dothiepin
10. Carbamazepine
11. Prazepam
12. Diltiazem
13. Pholcodine

## PHA 13 | Analysis of Blood Alcohol on BP20


**Column Part No.: 054442**

Phase: BP20, 1.0 µm film  
 Column: 25 m x 0.32 mm ID  
 Initial Temp: Isothermal, 60 °C  
 Detector: FID  
 Sensitivity: 64 x 10 -12 AFS  
 Injection Mode: Split

Note: The BP20 column allows the use of aqueous solutions.

**Components**

1. Acetone
2. Ethyl Acetate
3. Methanol
4. iso-Propanol
5. Ethanol
6. n-Propanol

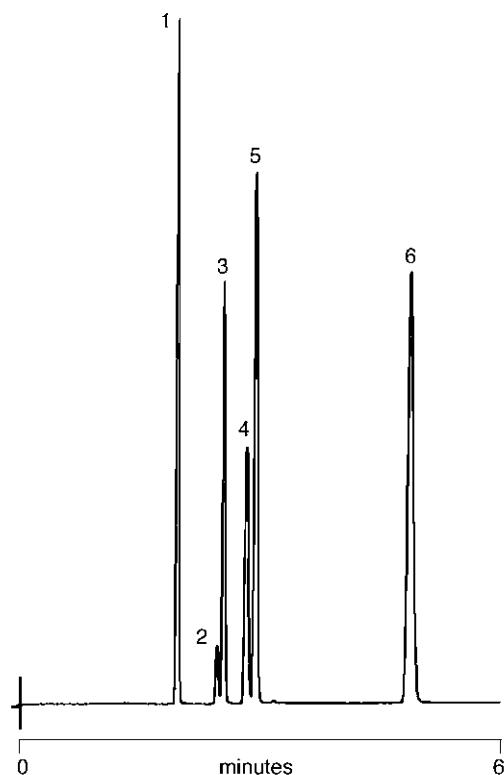


## PHA 06 | Analysis of Basic Drug Screen on BPX5 (10-20 ng/component)

### Column Part No.: 054131

Phase:	BPX5, 1.0 $\mu\text{m}$	Final Temp.:	310 °C
Column:	25 m x 0.53 mm I.D.	Detector:	FID
Initial Temp.:	120 °C	Injector:	Split, 240 °C
Rate:	10 °C/min	Carrier Gas:	H <sub>2</sub> , 2 psi

Note: The low bleed nature of the BPX5 allows trace analysis to be performed.

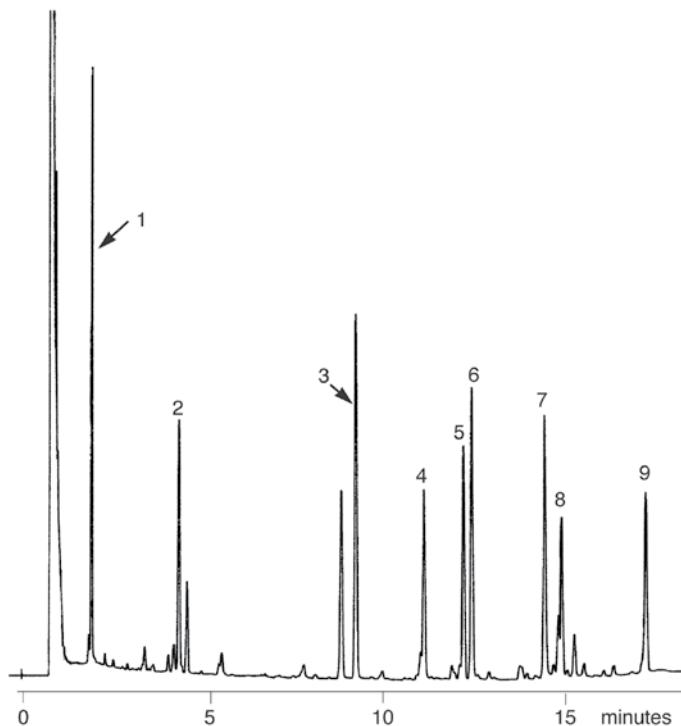


### Components

1. Methamphetamine
2. Phenidimetrazine
3. Phencyclidine
4. Mepivacaine
5. Methaqualone
6. Amitriptyline
7. Codeine
8. Diazepam
9. Fentanyl

## PHA 08 | Underivatized Steroid Analysis on BPX5

### Column Part No.: 054113

Phase:	BPX5, 0.25 $\mu\text{m}$
Column:	25 m x 0.22 mm ID
Initial Temp.:	180 °C
Rate:	8 °C/min
Final Temp.:	350 °C, 10 min
Detector:	FID
Sensitivity:	32 x 10 -12 AFS
Injection Mode:	Split
Carrier Gas:	H <sub>2</sub> , 10 psi

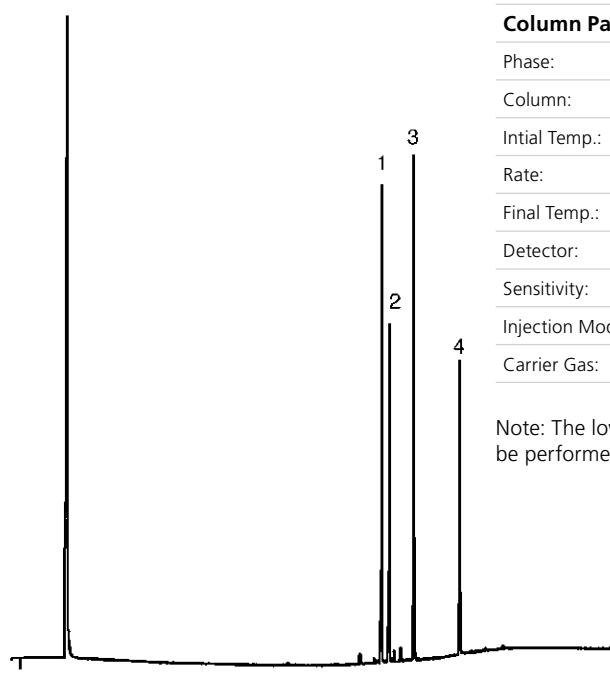

Note: The low bleed nature of the BPX5 allows trace analysis to be performed.

### Components


1. Testosterone
2. Pregnenolone
3. Progesterone
4. Cholesterol



GC Columns and Applications



## GC Columns and Applications

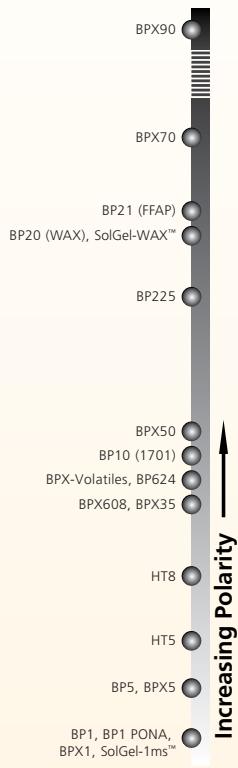


## PHA 15 | Analysis of Horse Racing Test Mix on BPX5

Column Part No.:	054101
Phase:	BPX5, 0.25 µm film
Column:	30 m x 0.25 mm ID
Horse Racing standard*:	10 ppm in methanol
Initial Temp:	75 °C, 2 min
Rate 1:	15 °C/min to 300 °C
Rate 2:	20 °C/min to 320 °C
Final Temp:	320 °C, 8 min.
Detector Type:	Mass Spectrometer
Carrier Gas:	He, 14.5 psi
Carrier Gas Flow:	1.5 mL/min


Constant Flow:	On
Average Linear Velocity:	45 cm/sec at 75 °C
Injection Mode:	Splitless
Purge on Time:	0.5 min
Purge on (Split)	
Vent Flow:	60 mL/min
Injection Volume:	1 µL
Injection Temperature:	250 °C
Liner Type:	4 mm ID Double Taper Liner
Liner Part Number:	092018

**Components**

6. Trimipramine
7. Phenytoin
8. Diazepam
9. Nordiazepam
10. Diphenoxylate
1. Metronidazole
2. Amylobarbitone
3. Pentobarbitone
4. Caffeine
5. Diphenhydramine

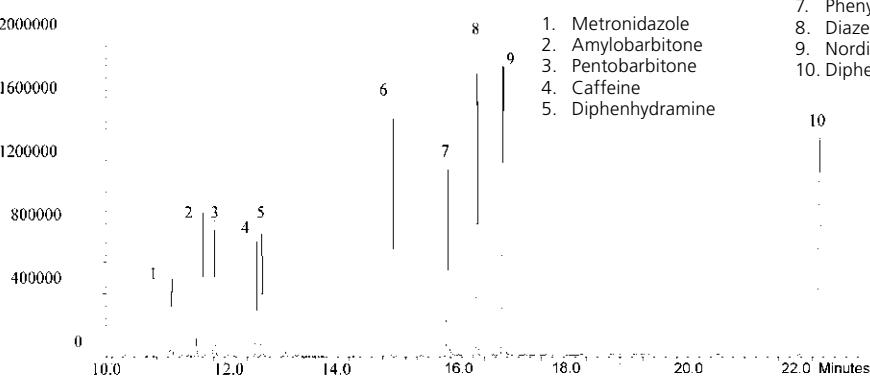

## PHA 03 | Analysis of Alkaloids on BP5

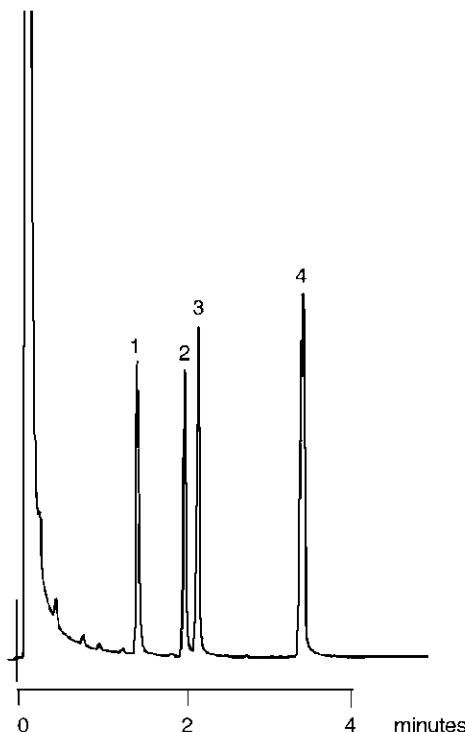**Column Part No.:** 054198

Phase:	BP5, 1.0 µm film
Column:	25 m x 0.53 mm ID
Initial Temp.:	200 °C, 0 min
Rate:	25 °C/min
Final Temp.:	300 °C, 0 min
Detector:	FID
Sensitivity:	128 x 10 -12 AFS
Injection Mode:	Split

Note: A 0.53 mm ID column can be used to screen samples rapidly.


**Components**

1. Cocaine
2. Codeine
3. Morphine
4. Quinine

## PHA 10 | Underivatized Barbiturates on BP5



GC Columns and Applications

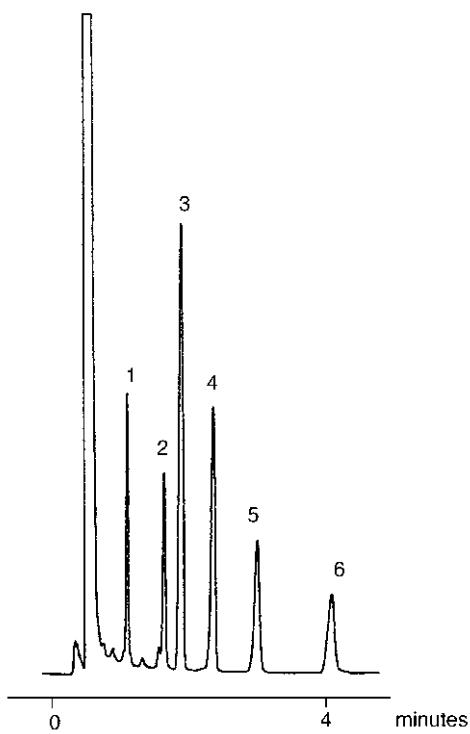


<b>Column Part No.:</b>	<b>054197</b>
Phase:	BP5, 1.0 µm
Column:	12 m x 0.53 mm I.D.
Temp:	195 °C
Carrier Gas:	Hydrogen
Carrier Flow:	10 mL/min
Injection Volume:	0.1 µL

Note: A 0.53 mm ID column can be used to screen samples rapidly.

### Components

1. Barbital
2. Butabarbital
3. Amobarbital
4. Pentobarbital
5. Secobarbital
6. Hexobarbital

## PHA 04 | Analysis of Sedatives/Hypnotics on BP1

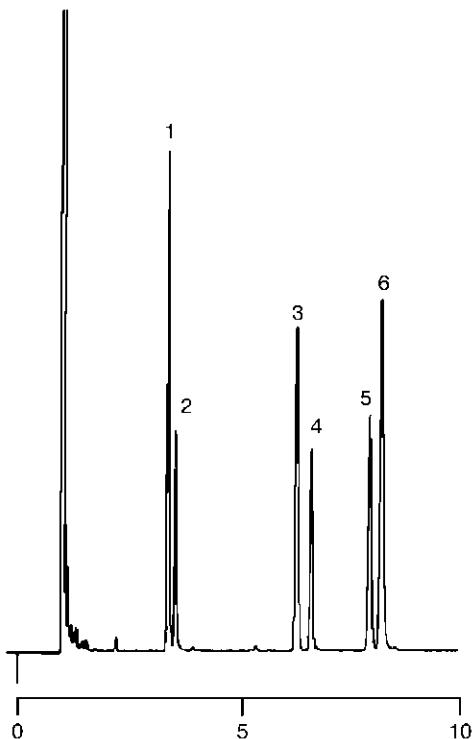

<b>Column Part No.:</b>	<b>054087</b>
Phase:	BP1, 1.0 µm film
Column:	25 m x 0.53 mm ID
Initial Temp.:	180 °C, 0 min
Rate:	10 °C/min
Final Temp.:	250 °C, 3 min
Detector:	FID
Sensitivity:	1024 x 10 -12 AFS
Injection Mode:	Split

### Components

1. Allobarbital
2. Aprobarbital
3. Diphenhydramine
4. Mephobarbital
5. Methapyrilene
6. Chloropheniramine



## PHA 01 | Analysis of Acid/Neutral Drugs on BPX35

Column Part No.:	054711		
Phase:	BPX35, 0.25 µm	Final Temp.:	300 °C, 5 min
Column:	25 m x 0.22 mm ID	Carrier Gas:	He, 150 kpa
Initial Temp.:	100 °C, 1 min	Injection Mode:	Split, (20:1)
Rate:	10 °C/min	Detector:	FID, 380 °C

Note: BPX35 is a low bleed column with a maximum temperature of 360 °C. Very compatible with GC/MS systems.

